

EXHIBIT D

(PART 1 OF 3)

US006565509B1

(12) **United States Patent**
Say et al.

(10) **Patent No.: US 6,565,509 B1**
 (45) **Date of Patent: May 20, 2003**

(54) **ANALYTE MONITORING DEVICE AND METHODS OF USE**

4,008,717 A 2/1977 Kowarski
 4,016,866 A 4/1977 Lawton

(List continued on next page.)

(75) Inventors: **James Say**, Alameda, CA (US);
Michael F. Tomasco, Cupertino, CA (US);
Adam Heller, Austin, TX (US);
Yoram Gal, Kibbutz Yagur (IL);
Behrad Aria, Alameda, CA (US);
Ephraim Heller, Oakland, CA (US);
Phillip John Plante, Sunnyvale, CA (US);
Mark S. Vreeke, Alameda, CA (US);
Keith A. Friedman, Austin, TX (US);
Fredric C. Colman, Berkeley, CA (US)

FOREIGN PATENT DOCUMENTS

DE 29 03 216 8/1979
 DE 227 029 A3 9/1985

(List continued on next page.)

OTHER PUBLICATIONS

Abruña, H. D. et al., "Rectifying Interfaces Using Two-Layer Films of Electrochemically Polymerized Vinylpyridine and Vinylbipyridine Complexes of Ruthenium and Iron on Electrodes," *J. Am. Chem. Soc.*, 103(1):1-5 (Jan. 14, 1981).

(List continued on next page.)

Primary Examiner—Max F. Hindenburg
Assistant Examiner—Navin Natnithithadha

(74) *Attorney, Agent, or Firm*—Merchant & Gould P.C.

(73) Assignee: **TheraSense, Inc.**, Alameda, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 104 days.

(21) Appl. No.: **09/667,199**

(22) Filed: **Sep. 21, 2000**

Related U.S. Application Data

(63) Continuation of application No. 09/070,677, filed on Apr. 30, 1998.

(51) Int. Cl.⁷ **A61B 5/00**; A61B 5/05

(52) U.S. Cl. **600/365**; 600/347; 600/345

(58) Field of Search 600/365, 345, 600/346, 347, 354, 357, 366, 309

(56) References Cited


U.S. PATENT DOCUMENTS

3,260,656 A 7/1966 Ross, Jr.
 3,653,841 A 4/1972 Klein
 3,719,564 A 3/1973 Lilly, Jr. et al.
 3,776,832 A 12/1973 Oswin et al.
 3,837,339 A 9/1974 Aisenberg et al.
 3,926,760 A 12/1975 Allen et al.
 3,972,320 A 8/1976 Kalman
 3,979,274 A 9/1976 Newman

(57) ABSTRACT

An analyte monitor includes a sensor, a sensor control unit, and a display unit. The sensor has, for example, a substrate, a recessed channel formed in the substrate, and conductive material disposed in the recessed channel to form a working electrode. The sensor control unit typically has a housing adapted for placement on skin and is adapted to receive a portion of an electrochemical sensor. The sensor control unit also includes two or more conductive contacts disposed on the housing and configured for coupling to two or more contact pads on the sensor. A transmitter is disposed in the housing and coupled to the plurality of conductive contacts for transmitting data obtained using the sensor. The display unit has a receiver for receiving data transmitted by the transmitter of the sensor control unit and a display coupled to the receiver for displaying an indication of a level of an analyte. The analyte monitor may also be part of a drug delivery system to alter the level of the analyte based on the data obtained using the sensor.

56 Claims, 26 Drawing Sheets

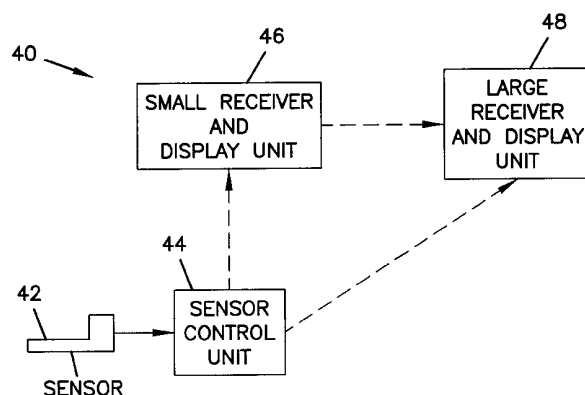

US 6,565,509 B1

Page 2

U.S. PATENT DOCUMENTS

4,055,175 A	10/1977	Clemens et al.	4,757,022 A	7/1988	Shults et al.
4,059,406 A	11/1977	Fleet	4,758,323 A	7/1988	Davis et al.
4,076,596 A	2/1978	Connery et al.	4,759,371 A	7/1988	Franetzki
4,098,574 A	7/1978	Dappen	4,759,828 A	7/1988	Young et al.
4,100,048 A	7/1978	Pompei et al.	4,764,416 A	8/1988	Ueyama et al.
4,151,845 A	5/1979	Clemens	4,776,944 A	10/1988	Janata et al.
4,168,205 A	9/1979	Danninger et al.	4,781,798 A	11/1988	Gough
4,172,770 A	10/1979	Semersky et al.	4,784,736 A	11/1988	Lonsdale et al.
4,178,916 A	12/1979	McNamara	4,795,707 A	1/1989	Niiyama et al.
4,206,755 A	6/1980	Klein	4,796,634 A	1/1989	Huntsman et al.
4,224,125 A	9/1980	Nakamura et al.	4,805,624 A	2/1989	Yao et al.
4,240,438 A	12/1980	Updike et al.	4,813,424 A	3/1989	Wilkins
4,247,297 A	1/1981	Berti et al.	4,815,469 A	3/1989	Cohen et al.
4,340,458 A	7/1982	Lerner et al.	4,820,399 A	4/1989	Senda et al.
4,352,960 A	10/1982	Dormer et al.	4,822,337 A	4/1989	Newhouse et al.
4,356,074 A	10/1982	Johnson	4,830,959 A	5/1989	McNeil et al.
4,365,637 A	12/1982	Johnson	4,832,797 A	5/1989	Vadgama et al.
4,366,033 A	12/1982	Richter et al.	RE32,947 E	6/1989	Dormer et al.
4,375,399 A	3/1983	Havas et al.	4,840,893 A	6/1989	Hill et al.
4,384,586 A	5/1983	Christiansen	4,848,351 A	7/1989	Finch
4,390,621 A	6/1983	Bauer	4,871,351 A	10/1989	Feingold
4,401,122 A	8/1983	Clark, Jr.	4,871,440 A	10/1989	Nagata et al.
4,404,066 A	9/1983	Johnson	4,874,500 A	10/1989	Madou et al.
4,418,148 A	11/1983	Oberhardt	4,890,620 A	1/1990	Gough
4,427,770 A	1/1984	Chen et al.	4,894,137 A	1/1990	Takizawa et al.
4,431,004 A	2/1984	Bessman et al.	4,897,162 A	1/1990	Lewandowski et al.
4,436,094 A	3/1984	Cerami	4,897,173 A	1/1990	Nankai et al.
4,440,175 A	4/1984	Wilkins	4,909,908 A	3/1990	Ross et al.
4,450,842 A	5/1984	Zick et al.	4,911,794 A	3/1990	Parce et al.
4,458,686 A	7/1984	Clark, Jr.	4,917,800 A	4/1990	Lonsdale et al.
4,461,691 A	7/1984	Frank	4,919,141 A	4/1990	Zier et al.
4,469,110 A	9/1984	Slama	4,919,767 A	4/1990	Vadgama et al.
4,477,314 A	10/1984	Richter et al.	4,923,586 A	5/1990	Katayama et al.
4,484,987 A	11/1984	Gough	4,927,516 A	5/1990	Yamaguchi et al.
4,522,690 A	6/1985	Venkatasetty	4,934,369 A	6/1990	Maxwell
4,524,114 A	6/1985	Samuels et al.	4,935,105 A	6/1990	Churchouse
4,526,661 A	7/1985	Steckhan et al.	4,935,345 A	6/1990	Guilbeau et al.
4,534,356 A	8/1985	Papadakis	4,938,860 A	7/1990	Wogoman
4,538,616 A	9/1985	Rogoff	4,944,299 A	7/1990	Silvian
4,543,955 A	10/1985	Schroeppe	4,950,378 A	8/1990	Nagata
4,545,382 A	10/1985	Higgins et al.	4,953,552 A	9/1990	DeMarzo
4,552,840 A	11/1985	Riffer	4,954,129 A	9/1990	Giuliani et al.
4,560,534 A	12/1985	Kung et al.	4,969,468 A	11/1990	Byers et al.
4,571,292 A	2/1986	Liu et al.	4,970,145 A	11/1990	Bennetto et al.
4,573,994 A	3/1986	Fischell et al.	4,974,929 A	12/1990	Curry
4,581,336 A	4/1986	Malloy et al.	4,986,271 A	1/1991	Wilkins
4,595,011 A	6/1986	Phillips	4,994,167 A	2/1991	Shults et al.
4,619,754 A	10/1986	Niki et al.	5,001,054 A	3/1991	Wagner
4,627,445 A	12/1986	Garcia et al.	5,050,612 A	9/1991	Matsumura
4,627,908 A	12/1986	Miller	5,058,592 A	10/1991	Whisler
4,633,878 A	1/1987	Bombardieri	5,070,535 A	12/1991	Hochmair et al.
4,637,403 A	1/1987	Garcia et al.	5,082,550 A	1/1992	Rishpon et al.
4,650,547 A	3/1987	Gough	5,082,786 A	1/1992	Nakamoto
4,654,197 A	3/1987	Lilja et al.	5,089,112 A	2/1992	Skotheim et al.
4,655,880 A	4/1987	Liu	5,095,904 A	3/1992	Seligman et al.
4,655,885 A	4/1987	Hill et al.	5,101,814 A	4/1992	Palti
4,671,288 A	6/1987	Gough	5,108,564 A	4/1992	Szuminsky et al.
4,679,562 A	7/1987	Luksha	5,109,850 A	5/1992	Blanco et al.
4,680,268 A	7/1987	Clark, Jr.	5,120,420 A	6/1992	Nankai et al.
4,682,602 A	7/1987	Prohaska	5,126,034 A	6/1992	Carter et al.
4,684,537 A	8/1987	Graetzel et al.	5,133,856 A	7/1992	Yamaguchi et al.
4,685,463 A	8/1987	Williams	5,135,003 A	8/1992	Souma
4,703,756 A	11/1987	Gough et al.	5,141,868 A	8/1992	Shanks et al.
4,711,245 A	12/1987	Higgins et al.	5,161,532 A	11/1992	Joseph
4,717,673 A	1/1988	Wrighton et al.	5,165,407 A	11/1992	Wilson et al.
4,721,601 A	1/1988	Wrighton et al.	5,174,291 A	12/1992	Schoonen et al.
4,721,677 A	1/1988	Clark, Jr.	5,190,041 A	3/1993	Palti
4,726,378 A	2/1988	Kaplan	5,192,416 A	3/1993	Wang et al.
4,726,716 A	2/1988	McGuire	5,198,367 A	3/1993	Aizawa et al.
4,731,726 A	3/1988	Allen, III	5,202,261 A	4/1993	Musho et al.
			5,205,920 A	4/1993	Oyama et al.

US 6,565,509 B1

Page 3

5,208,154 A	5/1993	Weaver et al.	5,820,622 A	10/1998	Gross et al.
5,209,229 A	5/1993	Gilli	5,822,715 A	10/1998	Worthington et al.
5,217,595 A	6/1993	Smith et al.	5,827,184 A	10/1998	Netherly et al.
5,229,282 A	7/1993	Yoshioka et al.	5,840,020 A	11/1998	Heinonen et al.
5,250,439 A	10/1993	Musho et al.	5,842,983 A	12/1998	Abel et al.
5,262,035 A	11/1993	Gregg et al.	5,885,211 A	3/1999	Eppstein et al.
5,262,305 A	11/1993	Heller et al.	5,899,855 A	5/1999	Brown
5,264,103 A	11/1993	Yoshioka et al.	5,954,685 A	9/1999	Tierney
5,264,104 A	11/1993	Gregg et al.	5,971,922 A	10/1999	Arita et al.
5,264,106 A	11/1993	McAleer et al.	6,001,067 A	* 12/1999	Shults et al. 600/345
5,271,815 A	12/1993	Wong	6,024,699 A	2/2000	Surwit et al.
5,279,294 A	1/1994	Anderson et al.	6,122,351 A	9/2000	Schlueter, Jr. et al.
5,286,362 A	2/1994	Hoenes et al.	FOREIGN PATENT DOCUMENTS		
5,286,364 A	2/1994	Yacynych et al.	DE	3934299	10/1990
5,288,636 A	2/1994	Pollmann et al.	EP	0 010 375 A1	4/1980
5,293,546 A	3/1994	Tadros et al.	EP	0 026 995 A1	4/1981
5,320,098 A	6/1994	Davidson	EP	0 048 090 A2	3/1982
5,320,725 A	6/1994	Gregg et al.	EP	0 078 636 A1	5/1983
5,322,063 A	6/1994	Allen et al.	EP	0 096 288 A1	12/1983
5,337,747 A	8/1994	Neffel	EP	0 125 139 A2	11/1984
5,352,348 A	10/1994	Young et al.	EP	0 127 958 A2	12/1984
5,356,786 A	10/1994	Heller et al.	EP	0 136 362 A1	4/1985
5,368,028 A	11/1994	Palti	EP	0 170 375 A2	2/1986
5,372,133 A	12/1994	Hogen Esch	EP	0 177 743 A2	4/1986
5,376,251 A	12/1994	Kaneko et al.	EP	0 080 304 B1	5/1986
5,378,628 A	1/1995	Grätzel et al.	EP	0 184 909 A2	6/1986
5,387,327 A	2/1995	Khan	EP	0 206 218 A2	12/1986
5,390,671 A	2/1995	Lord et al.	EP	0 230 472 A1	8/1987
5,391,250 A	2/1995	Cheney, II et al.	EP	0 241 309 A3	10/1987
5,395,504 A	3/1995	Saurer et al.	EP	0 245 073 A2	11/1987
5,400,782 A	3/1995	Beaubiah	EP	0 278 647 A2	8/1988
5,411,647 A	5/1995	Johnson et al.	EP	0 359 831 A1	3/1990
5,437,999 A	8/1995	Diebold et al.	EP	0 368 209 A1	5/1990
5,469,846 A	11/1995	Khan	EP	0 390 390 A1	10/1990
5,491,474 A	2/1996	Suni et al.	EP	0 400 918 A1	12/1990
5,494,562 A	2/1996	Maley et al.	EP	0 453 283 A1	10/1991
5,496,453 A	3/1996	Uenoyama et al.	EP	0 470 290 A1	2/1992
5,497,772 A	3/1996	Schulman et al.	EP	0 127 958 B2	3/1992
5,531,878 A	7/1996	Vadgama et al.	EP	0 255 291 B1	6/1992
5,545,191 A	8/1996	Mann et al.	GB	1394171	5/1975
5,560,357 A	10/1996	Faupel et al.	GB	1599241 A	9/1981
5,562,713 A	10/1996	Silvian	GB	2 073 891 A	10/1981
5,565,085 A	10/1996	Ikeda et al.	GB	2 154 003 B	2/1988
5,567,302 A	10/1996	Song et al.	GB	2 204 408 A	11/1988
5,568,806 A	10/1996	Cheney, II et al.	GB	2 254 436 A	10/1992
5,569,186 A	10/1996	Lord et al.	JP	54-41191	4/1979
5,582,184 A	12/1996	Erickson et al.	JP	55-10581	1/1980
5,582,697 A	12/1996	Ikeda et al.	JP	55-10583	1/1980
5,582,698 A	12/1996	Flaherty et al.	JP	55-10584	1/1980
5,586,553 A	12/1996	Halili et al.	JP	55-12406	1/1980
5,589,326 A	12/1996	Deng et al.	JP	56-163447	12/1981
5,593,852 A	1/1997	Heller et al.	JP	57-70448	4/1982
5,596,150 A	1/1997	Arndt et al.	JP	60-173457	9/1985
5,617,851 A	4/1997	Lipkovker	JP	60-173458	9/1985
5,628,890 A	5/1997	Carter et al.	JP	60-173459	9/1985
5,651,869 A	7/1997	Yoshioka et al.	JP	61-90050	5/1986
5,660,163 A	8/1997	Schulman et al.	JP	62-85855	4/1987
5,670,031 A	9/1997	Hintsche et al.	JP	62-114747	5/1987
5,680,858 A	10/1997	Hansen et al.	JP	63-58149	3/1988
5,682,233 A	10/1997	Brinda	JP	63-128252	5/1988
5,695,623 A	12/1997	Michel et al.	JP	63-139246	6/1988
5,708,247 A	1/1998	McAleer et al.	JP	63-294799	12/1988
5,711,001 A	1/1998	Iliff et al.	JP	63-317757	12/1988
5,711,861 A	* 1/1998	Ward et al. 204/403.09	JP	63-317758	12/1988
5,711,862 A	1/1998	Sakoda et al.	JP	1-114746	5/1989
5,741,211 A	4/1998	Renirie et al.	JP	1-114747	5/1989
5,771,001 A	6/1998	Cobb	JP	1-124060	5/1989
5,791,344 A	8/1998	Schulman et al.	JP	1-134244	5/1989
5,800,420 A	9/1998	Gross et al.	JP	1-156658	6/1989
5,807,375 A	9/1998	Gross et al.	JP	2-62958	3/1990
5,820,551 A	10/1998	Hill et al.			

US 6,565,509 B1

Page 4

JP	2-120655	5/1990
JP	2-287145	11/1990
JP	2-310457	12/1990
JP	3-26956	2/1991
JP	3-28752	2/1991
JP	3-202764	9/1991
JP	5-72171	3/1993
JP	5-196595	8/1993
JP	5-190050	7/1994
JP	7-55757 A	3/1995
JP	7-72585	3/1995
JP	8-285814 A	11/1996
JP	8-285815 A	11/1996
JP	9-21778 A	1/1997
JP	9-101280 A	4/1997
JP	9-285459 A	11/1997
JP	10-170471 A	6/1998
SU	1281988 A1	1/1987
WO	WO 85/05119	11/1985
WO	WO 89/08713	9/1989
WO	WO 90/05300	5/1990
WO	WO 90/05910	5/1990
WO	WO 91/01680	2/1991
WO	WO 91/04704	4/1991
WO	WO 91/15993	10/1991
WO	WO 92/13271	8/1992
WO	WO 94/20602	9/1994
WO	WO 94/27140	11/1994
WO	WO 96/30431	10/1996
WO	WO 97/02847	1/1997
WO	WO 97/19344	5/1997
WO	WO 97/42882	11/1997
WO	WO 97/42883	11/1997
WO	WO 97/42886	11/1997
WO	WO 97/42888	11/1997
WO	WO 97/43962	11/1997

OTHER PUBLICATIONS

Albery, W. J. et al., "Amperometric enzyme electrodes. Part II. Conducting salts as electrode materials for the oxidation of glucose oxidase," *J. Electroanal. Chem. Interfacial Electrochem.*, 194(2) (1 page—Abstract only) (1985).

Albery, W. J. et al., "Amperometric Enzyme Electrodes," *Phil. Trans. R. Soc. Lond.* B316:107–119 (1987).

Alcock, S. J. et al., "Continuous Analyte Monitoring to Aid Clinical Practice," *IEEE Engineering in Medicine and Biology*, 319–325 (1994).

Anderson, L. B. et al., "Thin-Layer Electrochemistry: Steady-State Methods of Studying Rate Processes," *J. Electroanal. Chem.*, 10:295–395 (1965).

Bartlett, P. N. et al., "Covalent Binding of Electron Relays to Glucose Oxidation," *J. Chem. Soc. Chem. Commun.*, 1603–1604 (1987).

Bartlett, P. N. et al., "Modification of glucose oxidase by tetrathiafulvalene," *J. Chem. Soc., Chem. Commun.*, 16 (1 page—Abstract only) (1990).

Bartlett, P. N. et al., "Strategies for the Development of Amperometric Enzyme Electrodes," *Biosensors*, 3:359–379 (1987/88).

Bindra, D.S. et al., "Design and in Vitro Studies of a Needle-Type Glucose Sensor for Subcutaneous Monitoring," *Anal. Chem.*, 63(17):1692–1696 (Sep. 1, 1991).

Bobbioni-Harsch, E. et al., "Lifespan of subcutaneous glucose sensors and their performances during dynamic glycaemia changes in rats," *J. Biomed. Eng.* 15:457–463 (1993).

Brandt, J. et al., "Covalent attachment of proteins to polysaccharide carriers by means of benzoquinone," *Biochim. Biophys. Acta*, 386(1) (1 page Abstract only) (1975).

Brownlee, M. et al., "A Glucose-Controlled Insulin-Delivery System: Semisynthetic Insulin Bound to Lectin," *Science*, 206(4423):1190–1191 (Dec. 7, 1979).

Cass, A.E.G. et al., "Ferricinium Ion As An Electron Acceptor for Oxido-Reductases," *J. Electroanal. Chem.*, 190:117–127 (1985).

Cass, A.E.G. et al., "Ferrocene-Mediated Enzyme Electrode for Amperometric Determination of Glucose," *Anal. Chem.*, 56(4):667–671 (Apr. 1984).

Castner, J. F. et al., "Mass Transport and Reaction Kinetic Parameters Determined Electrochemically for Immobilized Glucose Oxidase," *Biochemistry*, 23(10):2203–2210 (1984).

Claremont, D.J. et al., "Biosensors for Continuous In Vivo Glucose Monitoring," *IEEE Engineering in Medicine and Biology Society 10th Annual International Conference*, New Orleans, Louisiana, 3 pgs. (Nov. 4–7, 1988).

Clark, L.C. et al., "Differential Anodic Enzyme Polarography for the Measurement of Glucose," *Oxygen Transport to Tissue: Instrumentation, Methods, and Physiology*, 127–132 (1973).

Clark, L.C., Jr. et al., "Electrode Systems for Continuous Monitoring in Cardiovascular Surgery," *Annals New York Academy of Sciences*, pp. 29–45 (1962).

Clark, L.C. et al., "Long-term Stability of Electroenzymatic Glucose Sensors Implanted in Mice," *Trans. Am. Soc. Artif. Intern. Organs*, XXXIV:259–265 (1988).

Clarke, W. L., et al., "Evaluating Clinical Accuracy of Systems for Self-Monitoring of Blood Glucose," *Diabetes Care*, 10(5):622–628 (Sep.–Oct. 1987).

Csöregi, E. et al., "Design, Characterization, and One-Point in Vivo Calibration of a Subcutaneously Implanted Glucose Electrode," *Anal. Chem.* 66(19):3131–3138 (Oct. 1, 1994).

Csöregi, E. et al., "Design and Optimization of a Selective Subcutaneously Implantable Glucose Electrode Based on "Wired" Glucose Oxidase," *Anal. Chem.* 67(7):1240–1244 (Apr. 1, 1995).

Csöregi, E. et al., "On-Line Glucose Monitoring by Using Microdialysis Sampling and Amperometric Detection Based on "Wired" Glucose Oxidase in Carbon Paste," *Mikrochim. Acta*. 121:31–40 (1995).

Davis, G., "Electrochemical Techniques for the Development of Amperometric Biosensors," *Biosensors*, 1:161–178 (1985).

Degani, Y. et al., "Direct Electrical Communication between Chemically Modified Enzymes and Metal Electrodes. 1. Electron Transfer from Glucose Oxidase to Metal Electrodes via Electron Relays, Bound Covalently to the Enzyme," *J. Phys. Chem.*, 91(6):1285–1289 (1987).

Degani, Y. et al., "Direct Electrical Communication between Chemically Modified Enzymes and Metal Electrodes. 2. Methods for Bonding Electron-Transfer Relays to Glucose Oxidase and D-Amino-Acid Oxidase," *J. Am. Chem. Soc.*, 110(8):2615–2620 (1988).

Degani, Y. et al., "Electrical Communication between Redox Centers of Glucose Oxidase and Electrodes via Electrostatically and Covalently Bound Redox Polymers," *J. Am. Chem. Soc.*, 111:2357–2358 (1989).

US 6,565,509 B1

Page 5

- Denisevich, P. et al., "Unidirectional Current Flow and Charge State Trapping at Redox Polymer Interfaces on Bilayer Electrodes: Principles, Experimental Demonstration, and Theory," *J. Am. Chem. Soc.*, 103(16):4727-4737 (1981).
- Dicks, J. M., "Ferrocene modified polypyrrole with immobilised glucose oxidase and its application in amperometric glucose microbiosensors," *Ann. Biol. clin.*, 47:607-619 (1989).
- Engstrom, R.C., "Electrochemical Pretreatment of Glassy Carbon Electrodes," *Anal. Chem.*, 54(13):2310-2314 (Nov. 1982).
- Engstrom, R.C. et al., "Characterization of Electrochemically Pretreated Glassy Carbon Electrodes," *Anal. Chem.*, 56(2):136-141 (Feb. 1984).
- Ellis, C. D., "Selectivity and Directed Charge Transfer through an Electroactive Metallopolymer Film," *J. Am. Chem. Soc.*, 103(25):7480-7483 (1981).
- Feldman, B.J. et al., "Electron Transfer Kinetics at Redox Polymer/Solution Interfaces Using Microelectrodes and Twin Electrode Thin Layer Cells," *J. Electroanal. Chem.*, 194(1):63-81 (Oct. 10, 1985).
- Fischer, H. et al., "Intramolecular Electron Transfer Mediated by 4,4'-Bipyridine and Related Bridging Groups," *J. Am. Chem. Soc.*, 98(18):5512-5517 (Sep. 1, 1976).
- Foulds, N.C. et al., "Enzyme Entrapment in Electrically Conducting Polymers," *J. Chem. Soc., Faraday Trans 1.*, 82:1259-1264 (1986).
- Foulds, N.C. et al., "Immobilization of Glucose Oxidase in Ferrocene-Modified Pyrrole Polymers," *Anal. Chem.*, 60(22):2473-2478 (Nov. 15, 1988).
- Frew, J.E. et al., "Electron-Transfer Biosensors," *Phil. Trans. R. Soc. Lond.*, B316:95-106 (1987).
- Gorton, L. et al., "Selective detection in flow analysis based on the combination of immobilized enzymes and chemically modified electrodes," *Analytica Chimica Acta.*, 250:203-248 (1991).
- Gregg, B. A. et al., "Cross-Linked Redox Gels Containing Glucose Oxidase for Amperometric Biosensor Applications," *Analytical Chemistry*, 62(3):258-263 (Feb. 1, 1990).
- Gregg, B. A. et al., "Redox Polymer Films Containing Enzymes. 1. A Redox-Conducting Epoxy Cement: Synthesis, Characterization, and Electrocatalytic Oxidation of Hydroquinone," *J. Phys. Chem.*, 95(15):5970-5975 (1991).
- Hale, P.D. et al., "A New Class of Amperometric Biosensor Incorporating a Polymeric Electron-Transfer Mediator," *J. Am. Chem. Soc.*, 111(9):3482-3484 (1989).
- Harrison, D.J. et al., "Characterization of Perfluorosulfonic Acid Polymer Coated Enzyme Electrodes and a Miniaturized Integrated Potentiostat for Glucose Analysis in Whole Blood," *Anal. Chem.*, 60(19):2002-2007 (Oct. 1, 1988).
- Hawkrige, F. M. et al., "Indirect Coulometric Titration of Biological Electron Transport Components," *Analytical Chemistry*, 45(7):1021-1027 (Jun. 1973).
- Heller, A., "Amperometric biosensors based on three-dimensional hydrogel-forming epoxy networks," *Sensors and Actuators B*, 13-14:180-183 (1993).
- Heller, A., "Electrical Connection of Enzyme Redox Centers to Electrodes," *J. Phys. Chem.*, 96(9):3579-3587 (1992).
- Heller, A., "Electrical Wiring of Redox Enzymes," *Acc. Chem. Res.*, 23(5):129-134 (1990).
- Ianniello, R.M. et al., "Immobilized Enzyme Chemically Modified Electrode as an Amperometric Sensor," *Anal. Chem.*, 53(13):2090-2095 (Nov. 1981).
- Ianniello, R.M. et al., "Differential Pulse Voltammetric Study of Direct Electron Transfer in Glucose Oxidase Chemically Modified Graphite Electrodes," *Anal. Chem.*, 54(7):1098-1101 (Jun. 1981).
- Ikeda, T. et al., "Glucose oxidase-immobilized benzoquinone-carbon paste electrode as a glucose sensor," *Agric. Biol. Chem.*, 49(2) (1 page—Abstract only) (1985).
- Ikeda, T. et al., "Kinetics of Outer-Sphere Electron Transfers Between Metal Complexes in Solutions and Polymeric Films on Modified Electrodes," *J. Am. Chem. Soc.*, 103(25):7422-7425 (Dec. 16, 1981).
- Johnson, J. M. et al., "Potential-Dependent Enzymatic Activity in an Enzyme Thin-Layer Cell," *Anal. Chem.*, 54:1377-1383 (1982).
- Johnson, K. W. et al., "Reproducible Electrodeposition of Biomolecules for the Fabrication of Miniature Electroenzymatic Biosensors," *Sensors and Actuators B Chemical*, B5:85-89 (1991).
- Jönsson, G. et al., "An Amperometric Glucose Sensor Made by Modification of a Graphite Electrode Surface With Immobilized Glucose Oxidase and Adsorbed Mediator," *Biosensors*, 1:355-368 (1985).
- Josowicz, M. et al., "Electrochemical Pretreatment of Thin Film Platinum Electrodes," *J. Electrochem. Soc.*, 135(1):112-115 (Jan. 1988).
- Katakis, I. et al., "Electrostatic Control of the Electron Transfer Enabling Binding of Recombinant Glucose Oxidase and Redox Polyelectrolytes," *J. Am. Chem. Soc.*, 116(8):3617-3618 (1994).
- Katakis, I. et al., "L- α -Glycerophosphate and L-Lactate Electrodes Based on the Electrochemical "Wiring" of Oxidases," *Analytical Chemistry*, 64(9):1008-1013 (May 1, 1992).
- Kenausis, G. et al., "'Wiring' of glucose oxidase and lactate oxidase within a hydrogel made with poly(vinyl pyridine) complexed with [Os(4,4'-dimethoxy-2,2'-bipyridine)₂Cl]⁺²⁺," *J. Chem. Soc., Faraday Trans.*, 92(20):4131-4136 (1996).
- Koudelka, M. et al., "In-Vivo Behaviour of Hypodermically Implanted Microfabricated Glucose Sensors," *Biosensors & Bioelectronics*, 6(1):31-36 (1991).
- Kulys, J. et al., "Mediatorless peroxidase electrode and preparation of bienzyme sensors," *Bioelectrochemistry and Bioenergetics*, 24:305-311 (1990).
- Lager, W. et al., "Implantable Electrocatalytic Glucose Sensor," *Horm. Metab. Res.*, 26:526-530 (Nov. 1994).
- Lindner, E. et al., "Flexible (Kapton-Based) Microsensor Arrays of High Stability for Cardiovascular Applications," *J. Chem. Soc. Faraday Trans.*, 89(2):361-367 (Jan. 21, 1993).
- Maidan, R. et al., "Elimination of Electrooxidizable Interferant-Produced Currents in Amperometric Biosensors," *Analytical Chemistry*, 64(23):2889-2896 (Dec. 1, 1992).
- Mastrototaro, J.J. et al., "An Electroenzymatic Glucose Sensor Fabricated on a Flexible Substrate," *Sensors and Actuators B Chemical*, B5:139-144 (1991).
- McNeil, C. J. et al., "Thermostable Reduced Nicotinamide Adenine Dinucleotide Oxidase: Application to Amperometric Enzyme Assay," *Anal. Chem.*, 61(1):25-29 (Jan. 1, 1989).
- Miyawaki, O. et al., "Electrochemical and Glucose Oxidase Coenzyme Activity of Flavin Adenine Dinucleotide Covalently Attached to Glassy Carbon at the Adenine Amino Group," *Biochimica et Biophysica Acta*, 838:60-68 (1985).

US 6,565,509 B1

Page 6

- Moatti-Sirat, D. et al., "Evaluating *in vitro* and *in vivo* the interference of ascorbate and acetaminophen on glucose detection by a needle-type glucose sensor," *Biosensors & Bioelectronics*, 7(5):345-352 (1992).
- Moatti-Sirat, D. et al., "Reduction of acetaminophen interference in glucose sensors by a composite Nafion membrane: demonstration in rats and man," *Diabetologia*, 37(6) (1 page—Abstract only) (Jun. 1994).
- Moatti-Sirat, D. et al., "Towards continuous glucose monitoring: *in vivo* evaluation of a miniaturized glucose sensor implanted for several days in rat subcutaneous tissue," *Diabetologia*, 35(3) (1 page—Abstract only) (Mar. 1992).
- Nagy, G. et al., "A New Type of Enzyme Electrode: The Ascorbic Acid Eliminator Electrode," *Life Sciences*, 31(23):2611-2616 (1982).
- Nakamura, S. et al., "Effect of Periodate Oxidation on the Structure and Properties of Glucose Oxidase," *Biochimica et Biophysica Acta*, 445:294-308 (1976).
- Narazimhan, K. et al., "p-Benzoquinone activation of metal oxide electrodes for attachment of enzymes," *Enzyme Microb. Technol.*, 7(6) (1 page—Abstract only) (1985).
- Ohara, T. J. et al., "Glucose Electrodes Based on Cross-Linked $[\text{Os}(\text{bpy})_2\text{Cl}]^{+2+}$ Complexed Poly(1-vinylimidazole) Films," *Analytical Chemistry*, 65(23):3512-3516 (Dec. 1, 1993).
- Ohara, T. J., "Osmium Bipyridyl Redox Polymers Used in Enzyme Electrodes," *Platinum Metals Rev.*, 39(2):54-62 (Apr. 1995).
- Ohara, T. J. et al., "Wired" Enzyme Electrodes for Amperometric Determination of Glucose or Lactate in the Presence of Interfering Substances," *Analytical Chemistry*, 66(15):2451-2457 (Aug. 1, 1994).
- Olivier, C. N. et al., "In vivo Measurement of Carbon Dioxide Tension with a Miniature Electrode," *Pflugers Arch.* 373:269-272 (1978).
- Paddock, R. et al., "Electrocatalytic reduction of hydrogen peroxide via direct electron transfer from pyrolytic graphite electrodes to irreversibly adsorbed cytochrome *c* peroxidase," *J. Electroanal. Chem.*, 260:487-494 (1989).
- Palleschi, G. et al., "A Study of Interferences in Glucose Measurements in Blood by Hydrogen Peroxide Based Glucose Probes," *Anal. Biochem.*, 159:114-121 (1986).
- Pankratov, I. et al., "Sol-gel derived renewable-surface biosensors," *Journal of Electroanalytical Chemistry*, 393:35-41 (1995).
- Pathak, C. P. et al., "Rapid Photopolymerization of Immunoprotective Gels in Contact with Cells and Tissue," *J. Am. Chem. Soc.*, 114(21):8311-8312 (1992).
- Pickup, J., "Developing glucose sensors for *in vivo* use," *Tibtech*, 11: 285-289 (Jul. 1993).
- Pickup, J. C. et al., "In vivo molecular sensing in diabetes mellitus: an implantable glucose sensor with direct electron transfer," *Diabetologia*, 32(3):213-217 (1989).
- Pickup, J. et al., "Potentially-implantable, amperometric glucose sensors with mediated electron transfer: improving the operating stability," *Biosensors*, 4(2) (1 page—Abstract only) (1989).
- Pishko, M. V. et al., "Amperometric Glucose Microelectrodes Prepared Through Immobilization of Glucose Oxidase in Redox Hydrogels," *Anal. Chem.*, 63(20):2268-2272 (Oct. 15, 1991).
- Poitout, V. et al., "A glucose monitoring system for on line estimation in man of blood glucose concentration using a miniaturized glucose sensor implanted in the subcutaneous tissue and a wearable control unit," *Diabetologia*, 36(7) (1 page—Abstract only) (Jul. 1993).
- Poitout, V. et al., "Calibration in dogs of a subcutaneous miniaturized glucose sensor using a glucose meter for blood glucose determination," *Biosensors & Bioelectronics*, 7:587-592 (1992).
- Poitout, V. et al., "In vitro and in vivo evaluation in dogs of a miniaturized glucose sensor," *ASAIO Transactions*, 37(3) (1 page—Abstract only) (Jul.-Sep. 1991).
- Pollak, A. et al., "Enzyme Immobilization by Condensation Copolymerization into Cross-Linked Polyacrylamide Gels," *J. Am. Chem. Soc.*, 102(20):6324-6336 (1980).
- Reach, G. et al., "Can Continuous Glucose Monitoring Be Used for the Treatment of Diabetes?" *Analytical Chemistry*, 64(6):381-386 (Mar. 15, 1992).
- Rebrin, K. et al., "Automated Feedback Control of Subcutaneous Glucose Concentration in Diabetic Dogs," *Diabetologia*, 32(8):573-576 (Aug. 1989).
- Sakakida, M. et al., "Ferrocene-mediate needle-type glucose sensor covered with newly designed biocompatible membrane," *Sensors and Actuators B*, 13-14:319-322 (1993).
- Samuels, G. J. et al., "An Electrode-Supported Oxidation Catalyst Based on Ruthenium (IV). pH "Encapsulation" in a Polymer Film," *J. Am. Chem. Soc.*, 103(2):307-312 (1981).
- Sasso, S.V. et al., "Electropolymerized 1,2-Diaminobenzene as a Means to Prevent Interferences and Fouling and to Stabilize Immobilized Enzyme in Electrochemical Biosensors," *Anal. Chem.*, 62(11):1111-1117 (Jun. 1, 1990).
- Scheller, F. et al., "Enzyme electrodes and their application," *Phil. Trans. R. Soc. Lond.*, B 316:85-94 (1987).
- Schmehl, R.H. et al., "The Effect of Redox Site Concentration on the Rate of Mediated Oxidation of Solution Substrates by a Redox Copolymer Film," *J. Electroanal. Chem.*, 152:97-109 (Aug. 25, 1983).
- Shichiri, M. et al., "Glycaemic Control in Pancreatized Dogs with a Wearable Artificial Endocrine Pancreas," *Diabetologia*, 24(3):179-184 (Mar. 1983).
- Sittampalam, G. et al., "Surface-Modified Electrochemical Detector for Liquid Chromatography," *Anal. Chem.*, 55(9):1608-1610 (Aug. 1983).
- Soegijoko, S. et al., *Horm. Metab. Res., Suppl. Ser.*, 12 (1 page—Abstract only) (1982).
- Sprules, S. D. et al., "Evaluation of a New Disposable Screen-Printed Sensor Strip for the Measurement of NADH and Its Modification to Produce a Lactate Biosensor Employing Microliter Volumes," *Electroanalysis*, 8(6):539-543 (1996).
- Sternberg, F. et al., "Calibration Problems of Subcutaneous Glucosensors when Applied "In-Situ" in Man," *Horm. metab. Res.*, 26:524-525 (1994).
- Sternberg, R. et al., "Covalent Enzyme Coupling on Cellulose Acetate Membranes for Glucose Sensor Development," *Analytical Chemistry*, 60(24):2781-2786 (Dec. 15, 1998).
- Sternberg, R. et al., "Study and Development of Multilayer Needle-type Enzyme-based Glucose Microsensors," *Biosensors*, 4:27-40 (1988).
- Suckane, M., "Immobilization of glucose isomerase," *Zeitschrift für Allgemeine Mikrobiologie*, 22(8):565-576 (1982).

US 6,565,509 B1

Page 7

- Tajima, S. et al., "Simultaneous Determination of Glucose and 1,5-Anhydroglucitol", *Chemical Abstracts*, 111(25):394 111:228556g (Dec. 18, 1989).
- Tarasevich, M.R. "Bioelectrocatalysis", *Comprehensive Treatise of Electrochemistry*, 10 (Ch. 4):231-295 (1985).
- Tatsuma, T. et al., "Enzyme Monolayer- and Bilayer-Modified Tin Oxide Electrodes for the Determination of Hydrogen Peroxide and Glucose," *Anal. Chem.*, 61(21):2352-2355 (Nov. 1, 1989).
- Taylor, C. et al., "'Wiring' of glucose oxidase within a hydrogel made with polyvinyl imidazole complexed with [(OS-4,4'-dimethoxy-2,2'-bipyridine)Cl]⁺²⁺," *Journal of Electroanalytical Chemistry*, 396:511-515 (1995).
- Trojanowicz, M. et al., "Enzyme Entrapped Polypyrrole Modified Electrode for Flow-Injection Determination of Glucose," *Biosensors & Bioelectronics*, 5:149-156 (1990).
- Turner, A.P.F. et al., "Diabetes Mellitus: Biosensors for Research and Management", *Biosensors*, 1:85-115 (1985).
- Turner, R. F. B. et al., "A Biocompatible Enzyme Electrode for Continuous *in vivo* Glucose Monitoring in Whole Blood," *Sensors and Actuators*, B1(1-6):561-564 (Jan. 1990).
- Tuzhi, P. et al., "Constant Potential Pretreatment of Carbon Fiber Electrodes for In Vivo Electrochemistry", *Analytical Letters*, 24(6):935-945 (1991).
- Umaha, M., "Protein-Modified Electrochemically Active Biomaterial Surface," *U.S. Army Research Office Report*, (12 pages) (Dec. 1988).
- Urban, G. et al., "Miniaturized Thin-Film Biosensors Using Covalently Immobilized Glucose Oxidase", *Biosensors & Bioelectronics*, 6(7):555-562 (1991).
- Velho, G. et al., "In Vitro and In Vivo Stability of Electrode Potentials in Needle-Type Glucose Sensors", *Diabetes*, 38(2):164-171 (Feb. 1989).
- Velho, G. et al., "Strategies for calibrating a subcutaneous glucose sensor", *Biomed. Biochim. Acta*, 48(11/12):957-964 (1989).
- Von Woedtke, T. et al., "In Situ Calibration of Implanted Electrochemical Glucose Sensors," *Biomed. Biochim. Acta*, 48(11/12):943-952 (1989).
- Vreeke, M. S. et al., "Chapter 15: Hydrogen Peroxide Electrodes Based on Electrical Connection of Redox Centers of Various Peroxidases to Electrodes through a Three-Dimensional Electron-Relaying Polymer Network," *Diagnostic Biosensor Polymers*, 7 pgs. (Jul. 26, 1993).
- Vreeke, M. et al., "Hydrogen Peroxide and β -Nicotinamide Adenine Dinucleotide Sensing Amperometric Electrodes Based on Electrical Connection of Horseradish Peroxidase Redox Centers to Electrodes through a Three-Dimensional Electron Relaying Polymer Network," *Analytical Chemistry*, 64(24):3084-3090 (Dec. 15, 1992).
- Wang, J. et al., "Activation of Glassy Carbon Electrodes by Alternating Current Electrochemical Treatment", *Analytica Chimica Acta*, 167:325-334 (Jan. 1985).
- Wang, J. et al., "Amperometric biosensing of organic peroxides with peroxidase-modified electrodes," *Analytica Chimica Acta*. 254:81-88 (1991).
- Wang, D. L. et al., "Miniaturized Flexible Amperometric Lactate Probe", *Analytical Chemistry*, 65(8):1069-1073 (Apr. 15, 1993).
- Wang, J. et al., "Screen-Printable Sol-Gel Enzyme-Containing Carbon Inks," *Analytical Chemistry*, 68(15):2705-2708 (Aug. 1, 1996).
- Wang, J. et al., "Sol-Gel-Derived Metal-Dispersed Carbon Composite Amperometric Biosensors," *Electroanalysis*, 9(1):52-55 (1997).
- Williams, D.L. et al., "Electrochemical-Enzymatic Analysis of Blood Glucose and Lactate", *Anal. Chem.*, 42(1):118-121 (Jan. 1970).
- Wilson, G. S. et al., "Progress toward the Development of an Implantable Sensor for Glucose," *Clinical Chemistry*, 38(9):1613-1617 (1992).
- Yabuki, S. et al., "Electro-conductive Enzyme Membrane," *J. Chem. Soc. Chem. Commun*, 945-946 (1989).
- Yang, L. et al., "Determination of Oxidase Enzyme Substrates Using Cross-Flow Thin-Layer Amperometry," *Electroanalysis*, 8(8-9):716-721 (1996).
- Yao, S.J. et al., "The Interference of Ascorbate and Urea in Low-Potential Electrochemical Glucose Sensing", *Proceedings of the Twelfth Annual International Conference of the IEEE Engineering in Medicine and Biology Society*, 12(2):487-489 (Nov. 1-4, 1990).
- Yao, T. et al., "A Chemically-Modified Enzyme Membrane Electrode As An Amperometric Glucose Sensor," *Analytica Chimica Acta.*, 148:27-33 (1983).
- Ye, L. et al., "High Current Density "Wired " Quinoprotein Glucose Dehydrogenase Electrode," *Anal. Chem.*, 65(3):238-241 (Feb. 1, 1993).
- Yildiz, A. et al., "Evaluation of an Improved Thin-Layer Electrode," *Analytical Chemistry*, 40(70):1018-1024 (Jun. 1968).
- Zamzow, K. et al., New Wearable Continuous Blood Glucose Monitor (BGM) and Artificial Pancreas (AP), *Diabetes*, 39:5A(20) (May 1990).
- Zhang, Y. et al., "Application of cell culture toxicity tests to the development of implantable biosensors," *Biosensors & Bioelectronics*, 6:653-661 (1991).
- Zhang, Y. et al., "Elimination of the Acetaminophen Interference in an Implantable Glucose Sensor," *Anal. Chem.* 66:1183-1188 (1994).

* cited by examiner


U.S. Patent

May 20, 2003

Sheet 1 of 26

US 6,565,509 B1

FIG. 1

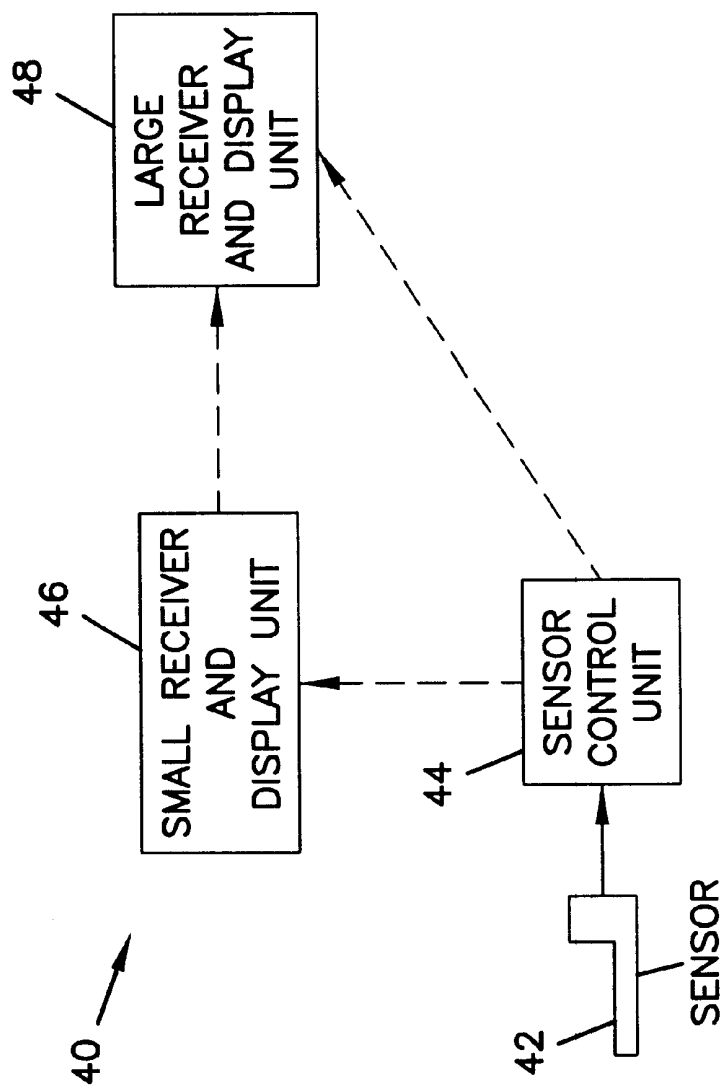


U.S. Patent

May 20, 2003

Sheet 2 of 26

US 6,565,509 B1

FIG. 2

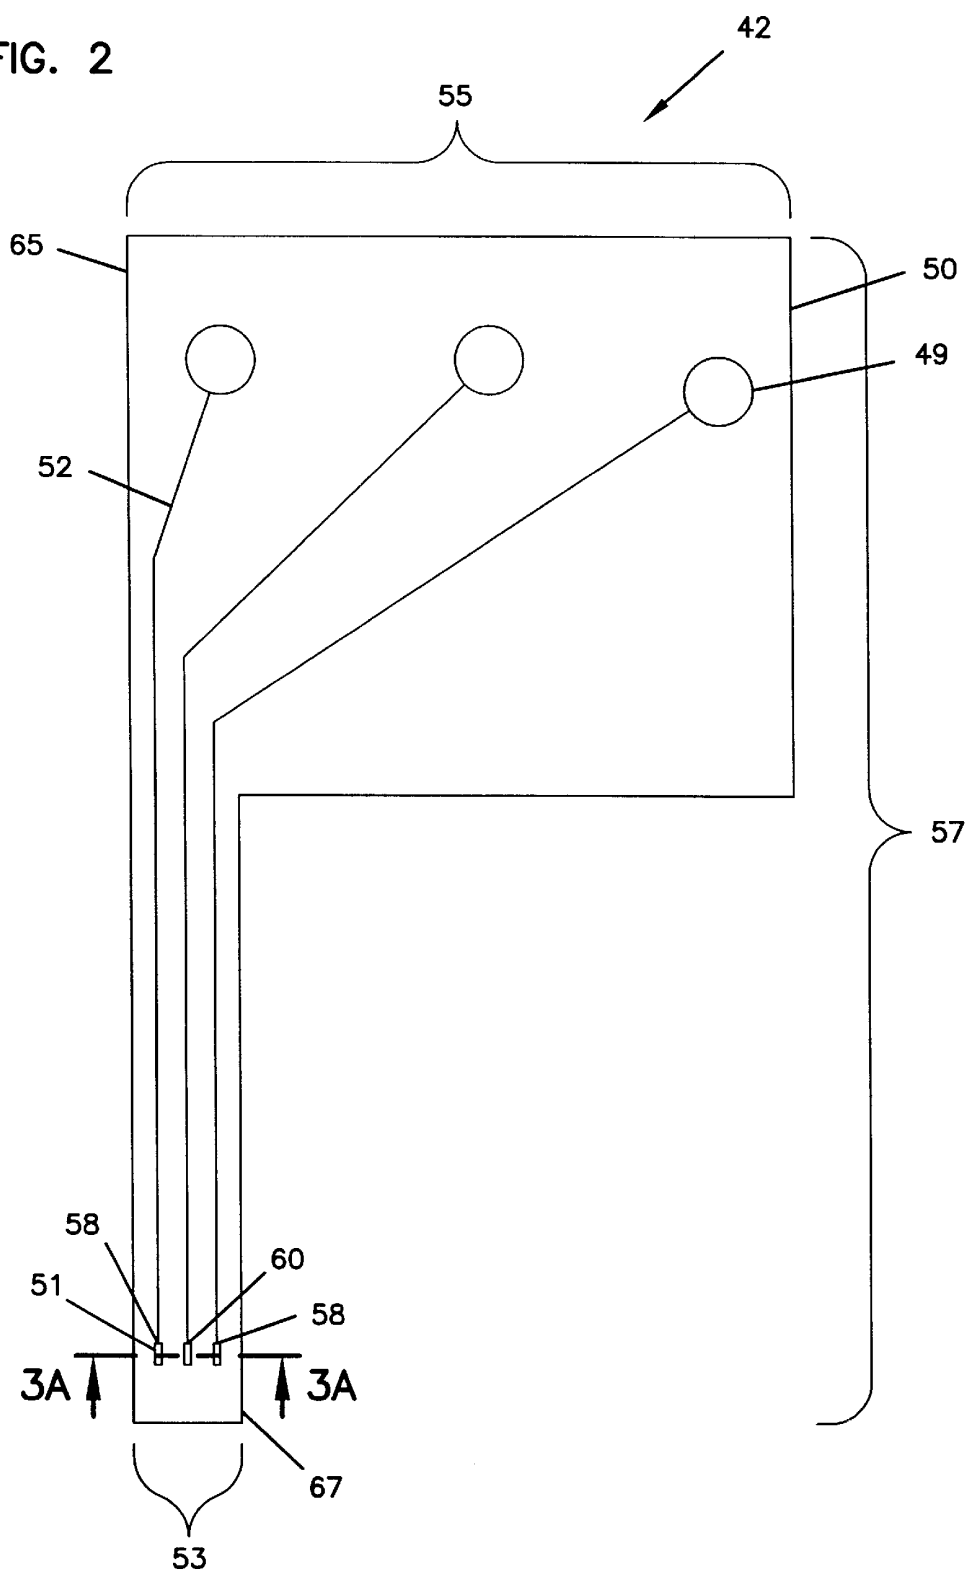

U.S. Patent

May 20, 2003

Sheet 3 of 26

US 6,565,509 B1

FIG. 3A

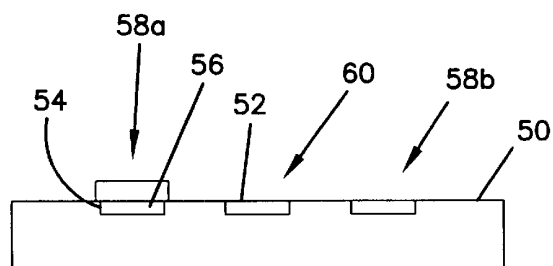


FIG. 3B

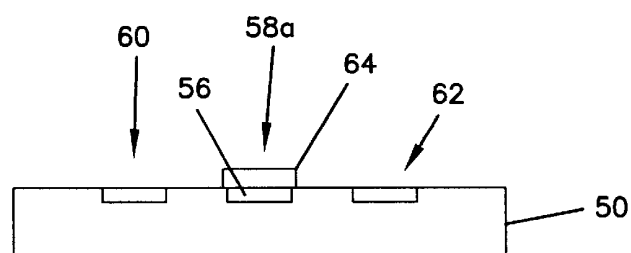


FIG. 9


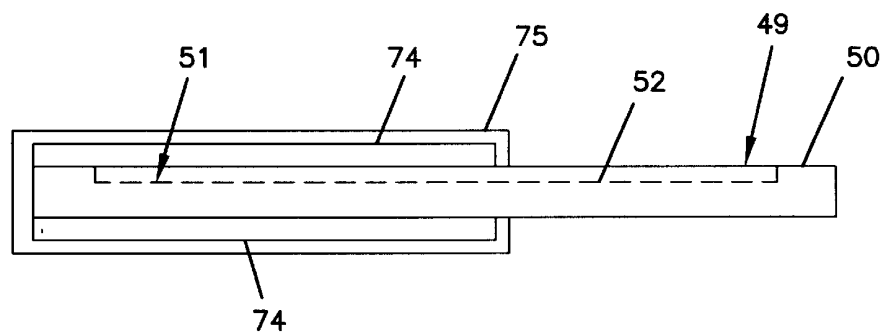


FIG. 4A

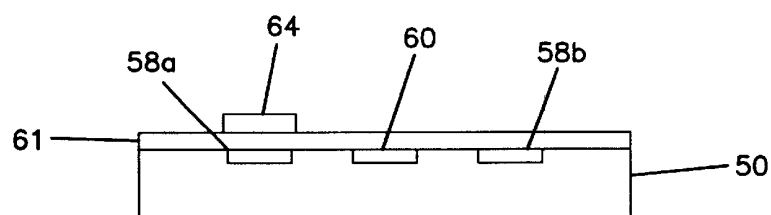

U.S. Patent

May 20, 2003

Sheet 4 of 26

US 6,565,509 B1

FIG. 4B


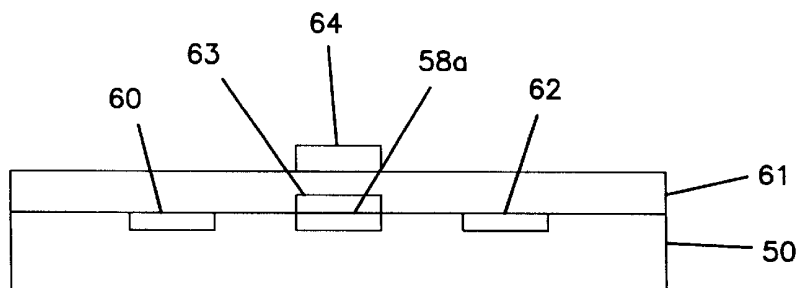


FIG. 5

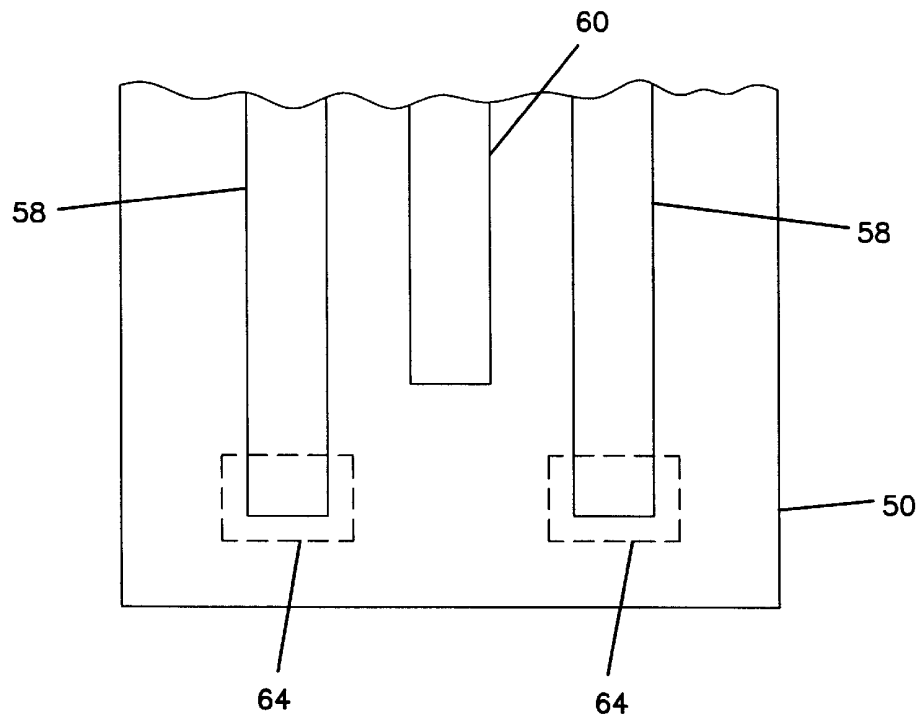

U.S. Patent

May 20, 2003

Sheet 5 of 26

US 6,565,509 B1

FIG. 6

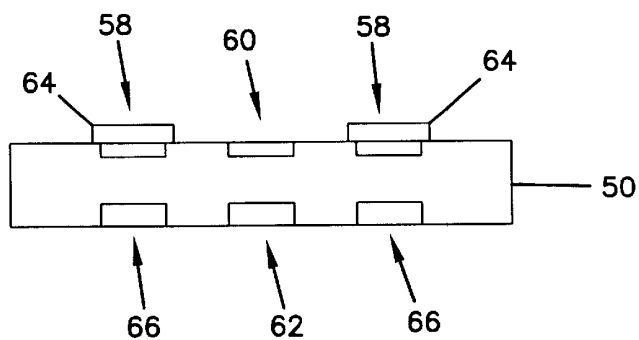


FIG. 7


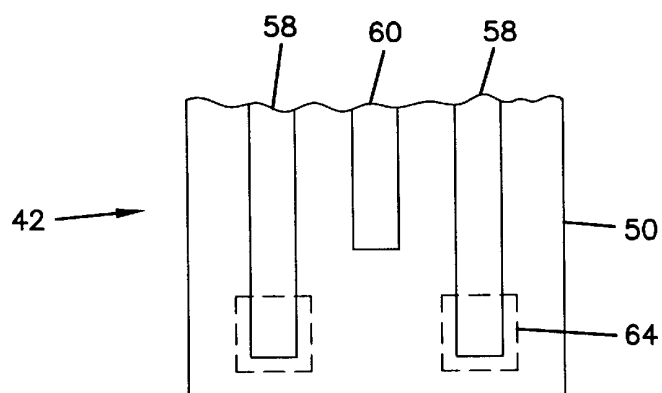


FIG. 8

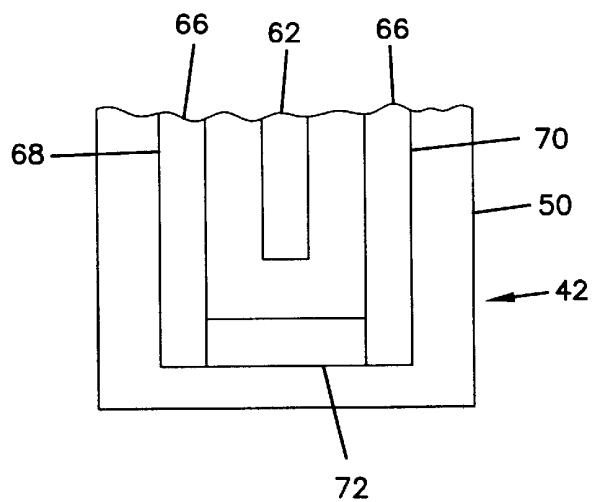


U.S. Patent

May 20, 2003

Sheet 6 of 26

US 6,565,509 B1

FIG. 10

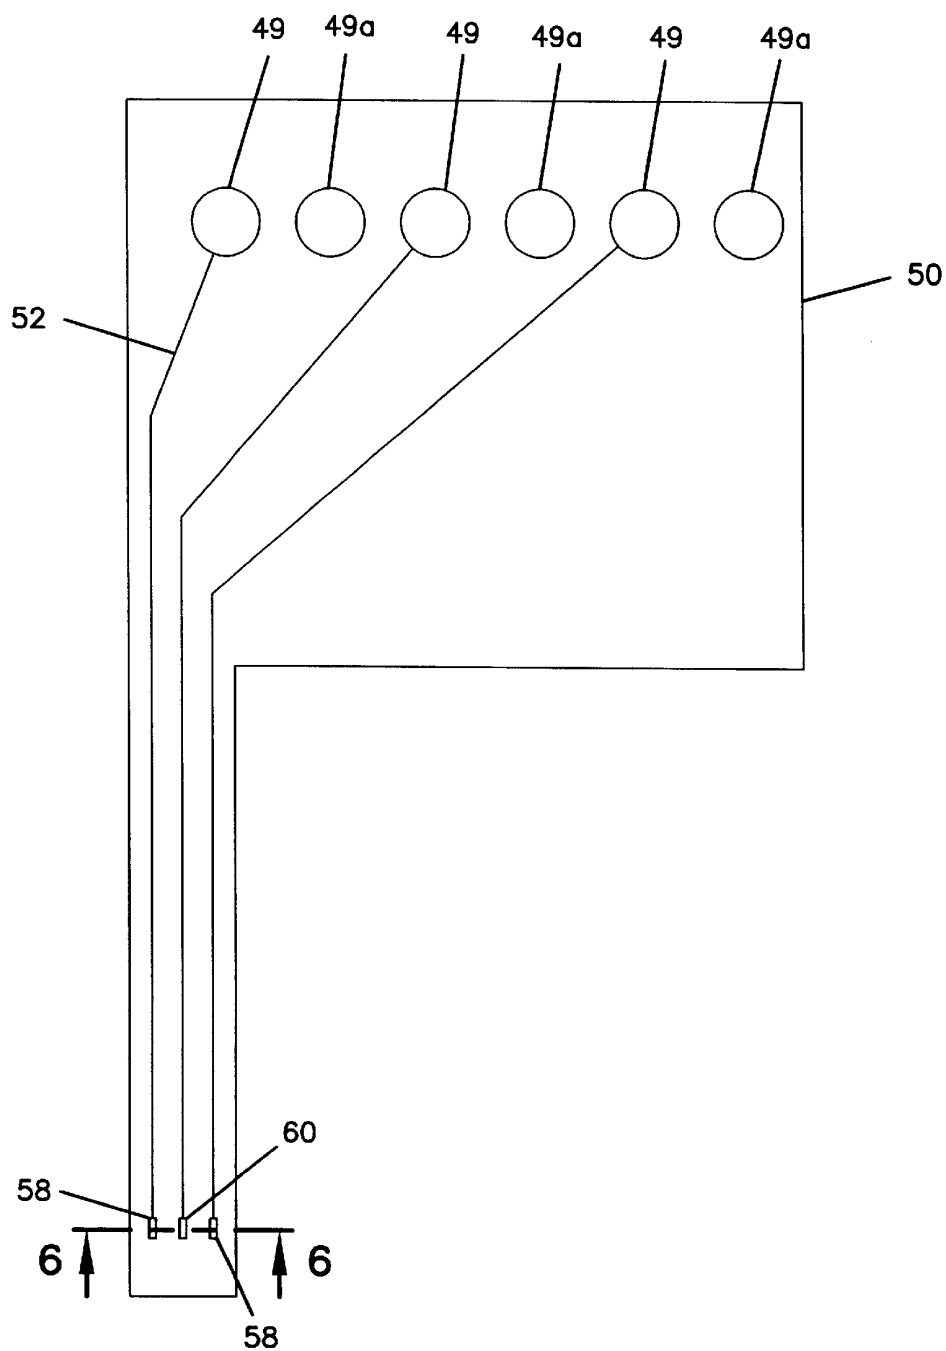


U.S. Patent

May 20, 2003

Sheet 7 of 26

US 6,565,509 B1

FIG. 11

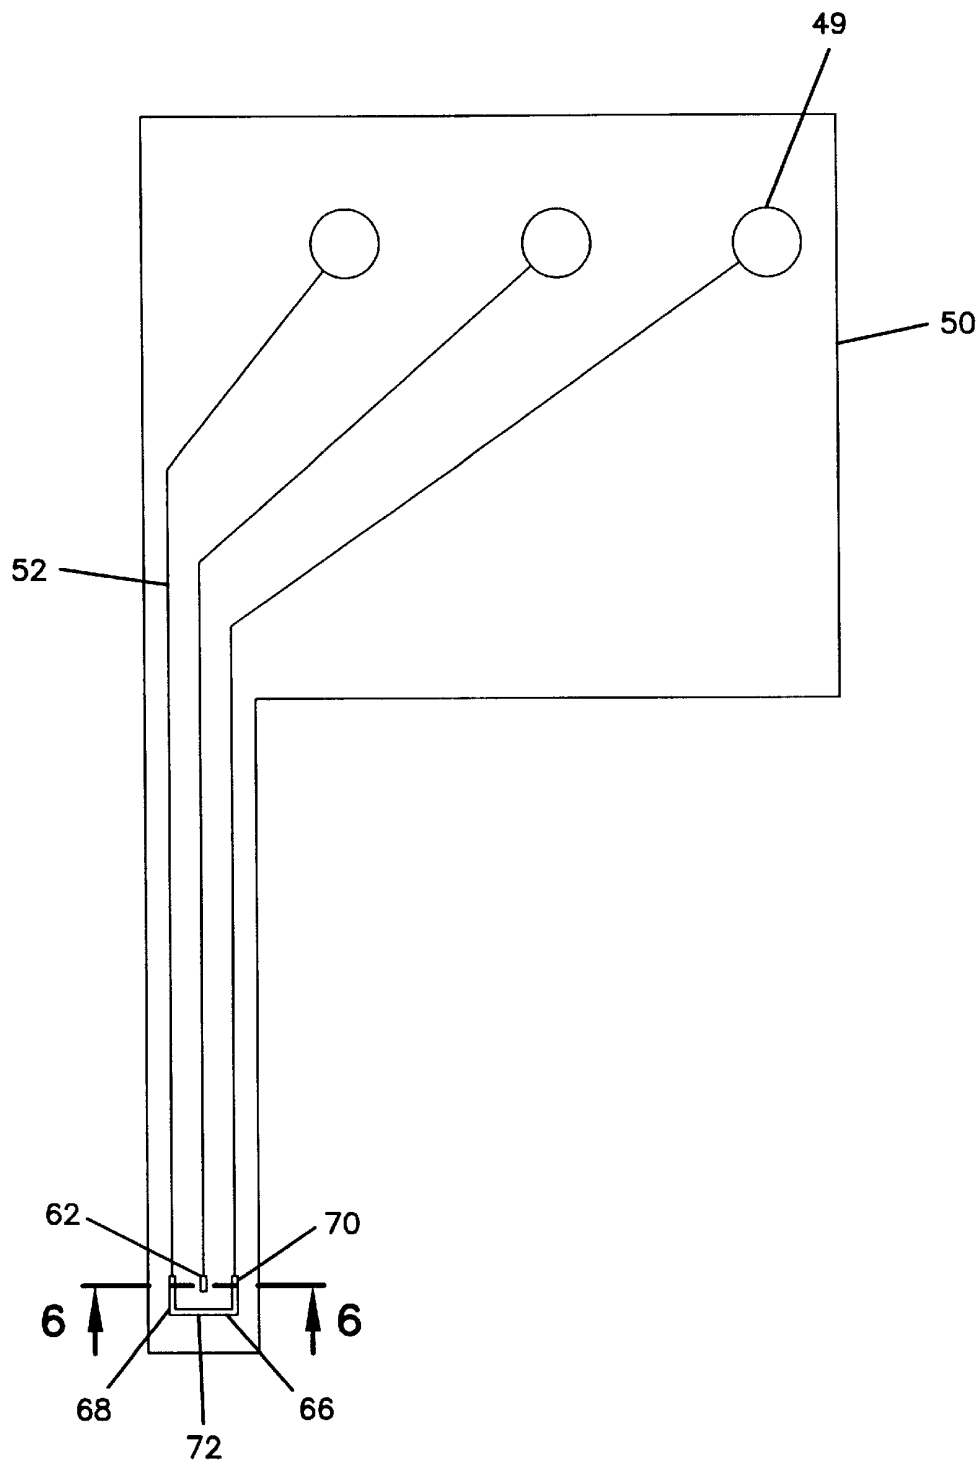

U.S. Patent

May 20, 2003

Sheet 8 of 26

US 6,565,509 B1

FIG. 12

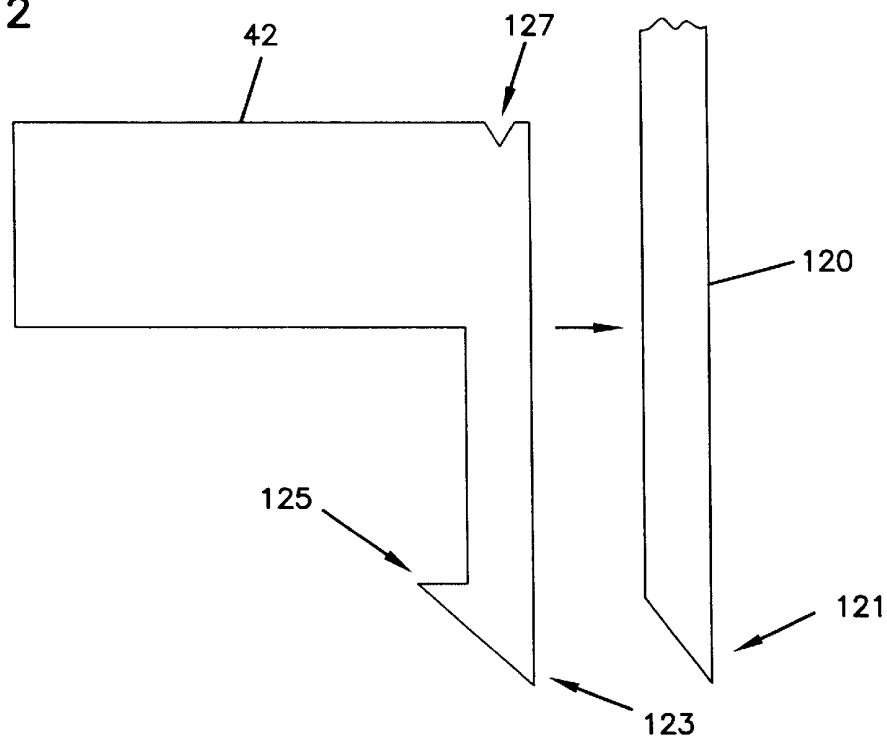


FIG. 13A




FIG. 13B


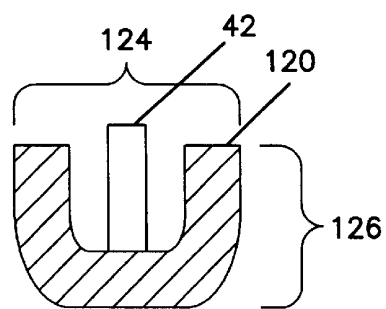


FIG. 13C

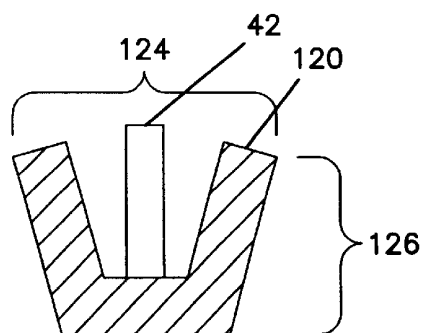

U.S. Patent

May 20, 2003

Sheet 9 of 26

US 6,565,509 B1

FIG. 15

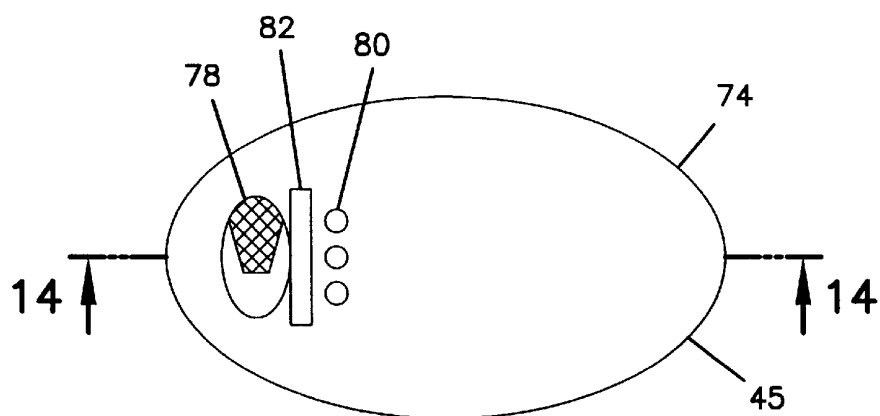


FIG. 16


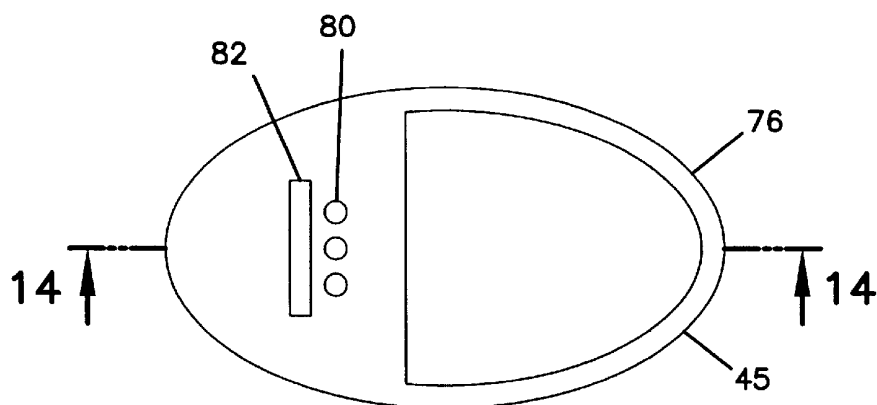


FIG. 14

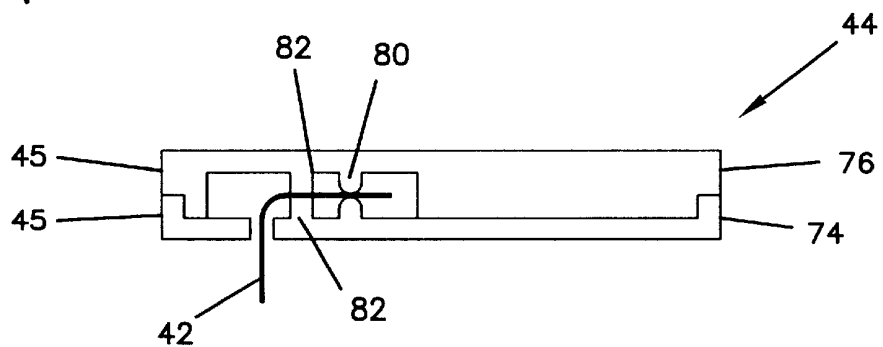


U.S. Patent

May 20, 2003

Sheet 10 of 26

US 6,565,509 B1

FIG. 17

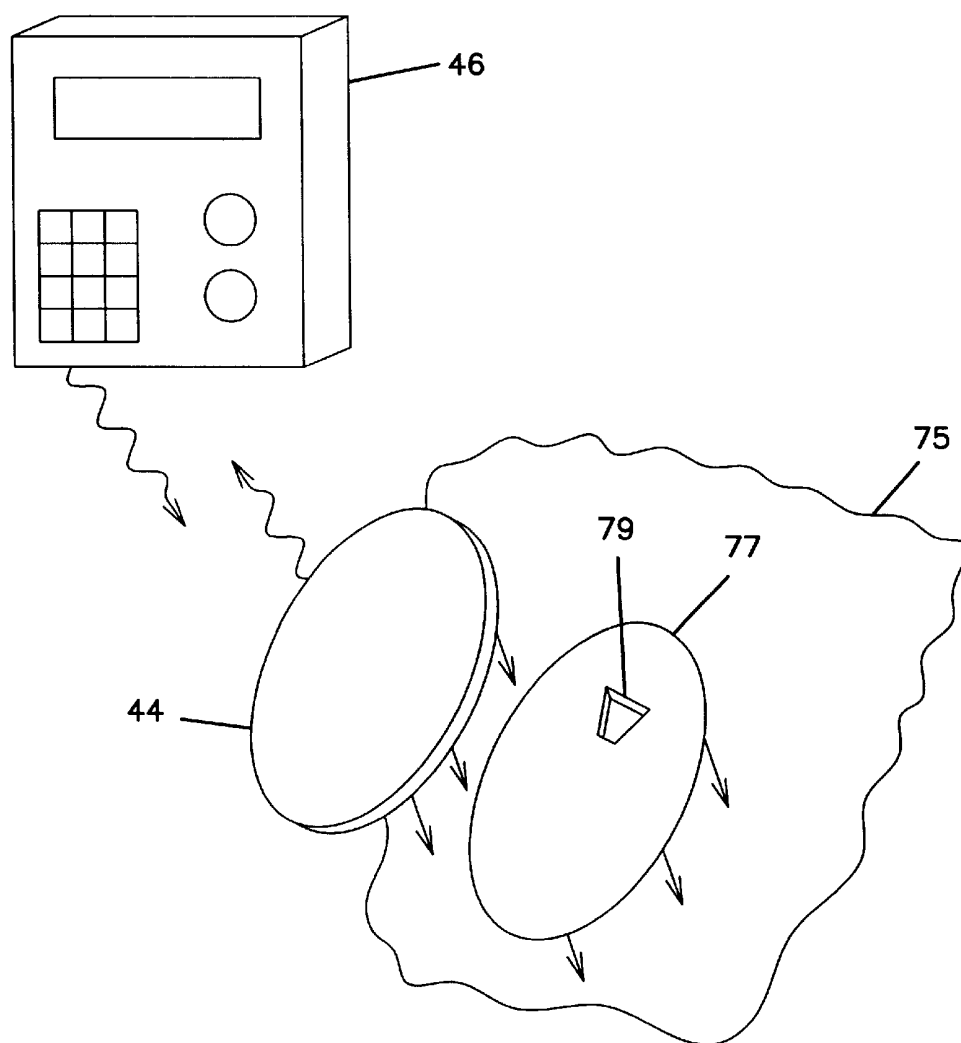


U.S. Patent

May 20, 2003

Sheet 11 of 26

US 6,565,509 B1

FIG. 18A

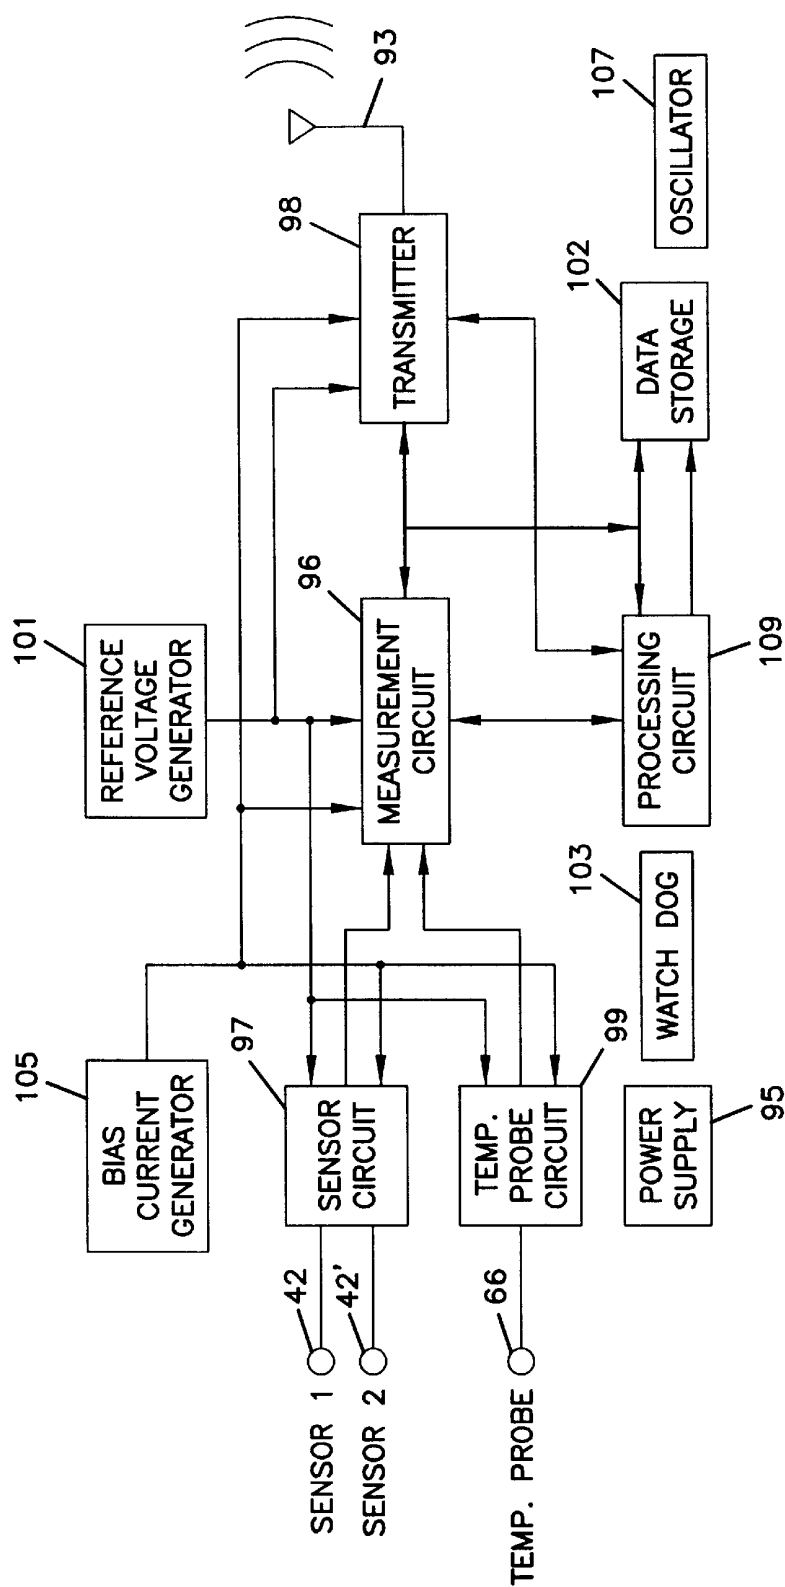


U.S. Patent

May 20, 2003

Sheet 12 of 26

US 6,565,509 B1

FIG. 18B

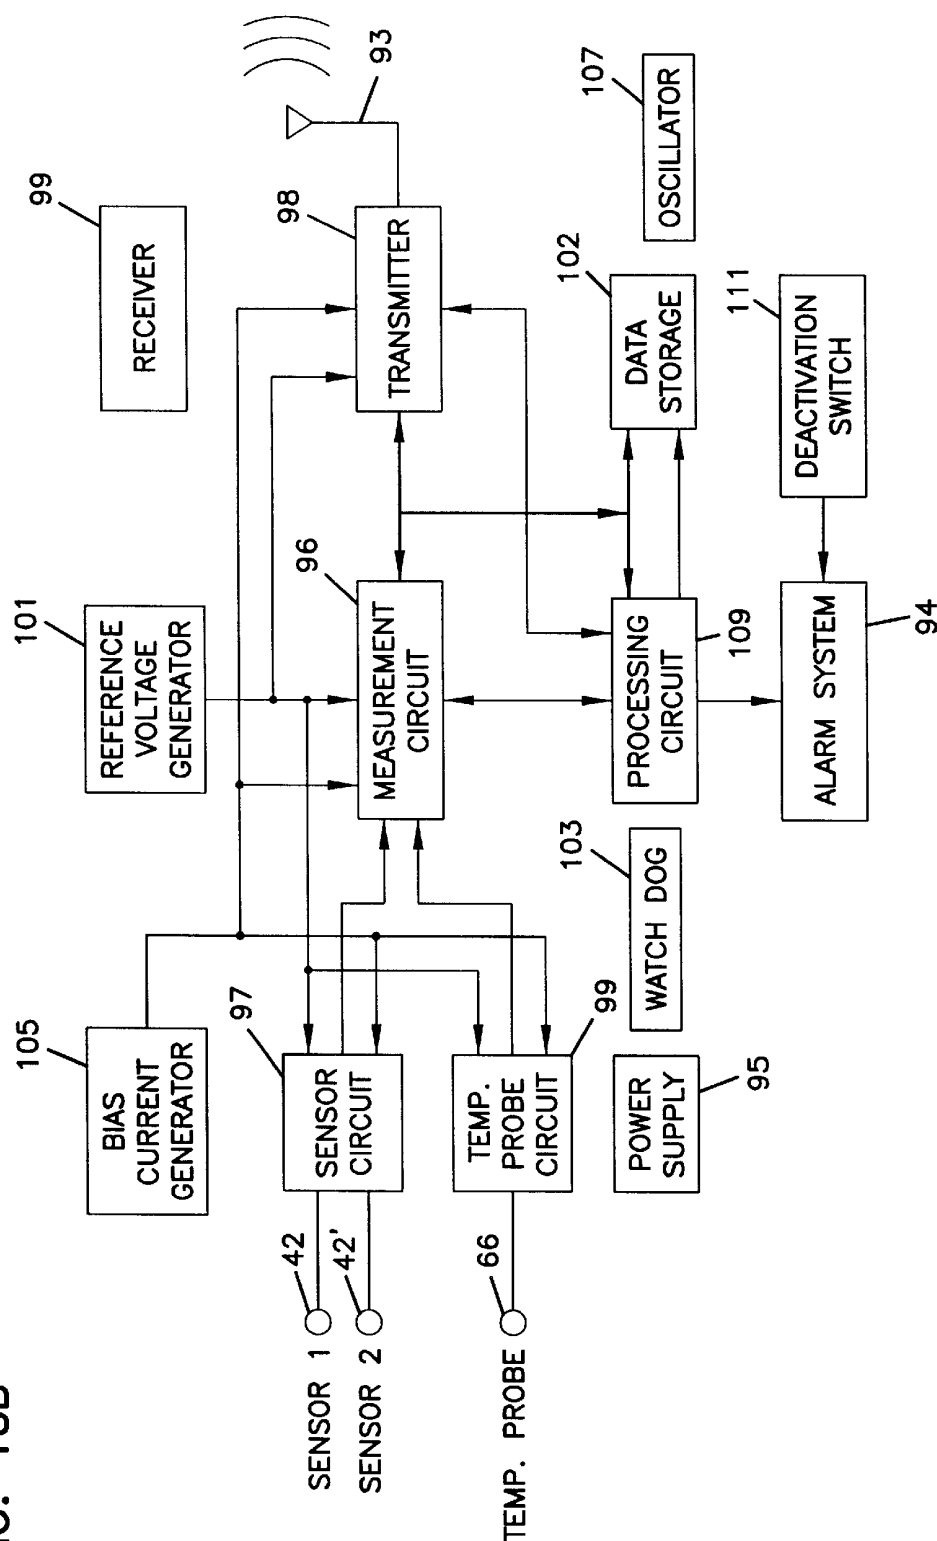

U.S. Patent

May 20, 2003

Sheet 13 of 26

US 6,565,509 B1

FIG. 19A

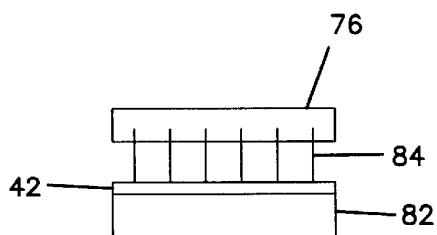


FIG. 19B

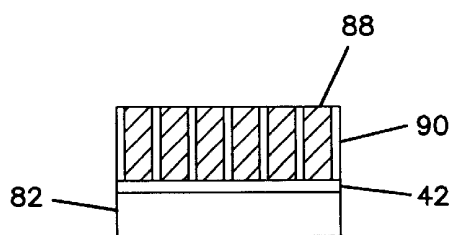


FIG. 19C

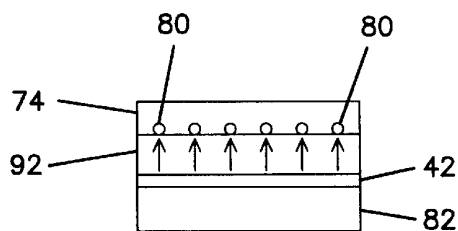


FIG. 19D

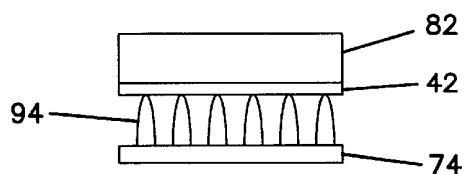


FIG. 19E


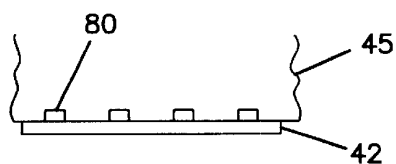


FIG. 19F

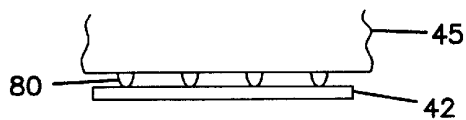

U.S. Patent

May 20, 2003

Sheet 14 of 26

US 6,565,509 B1

FIG. 20A

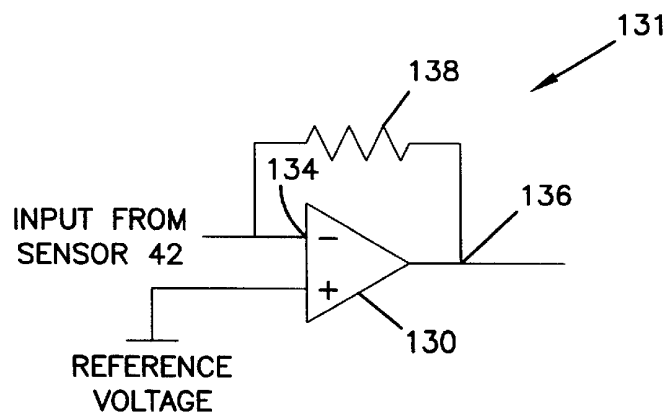


FIG. 20B


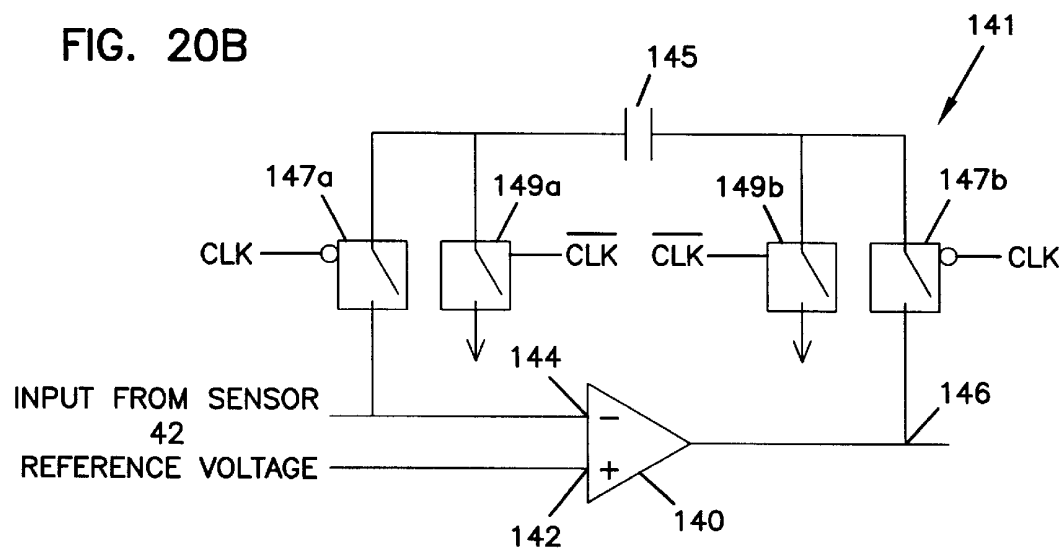


FIG. 21

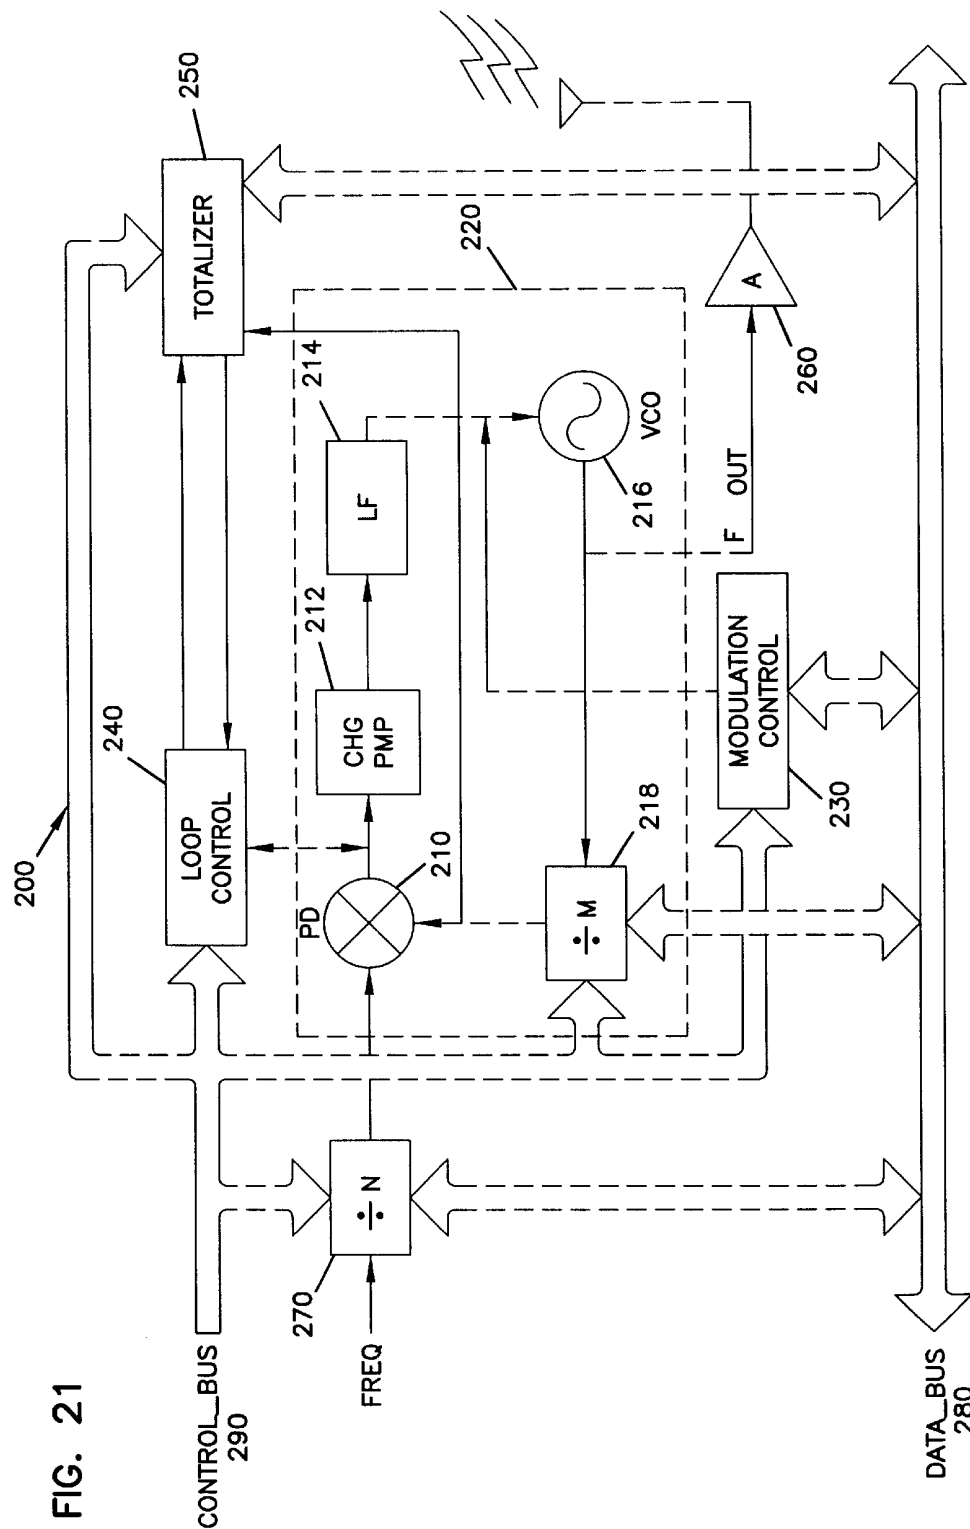


U.S. Patent

May 20, 2003

Sheet 16 of 26

US 6,565,509 B1

FIG. 22

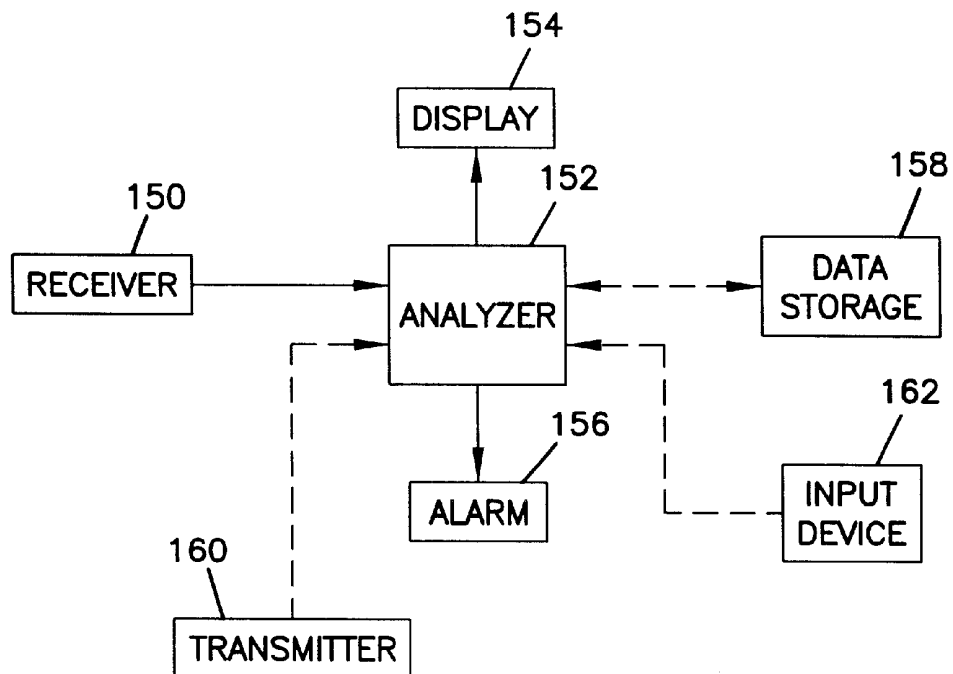

U.S. Patent

May 20, 2003

Sheet 17 of 26

US 6,565,509 B1

FIG. 23

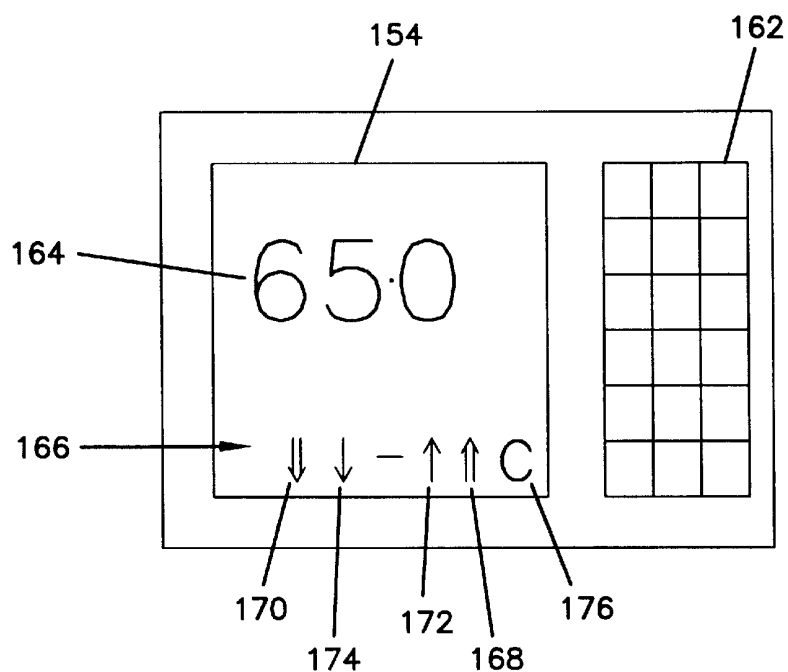


FIG. 24


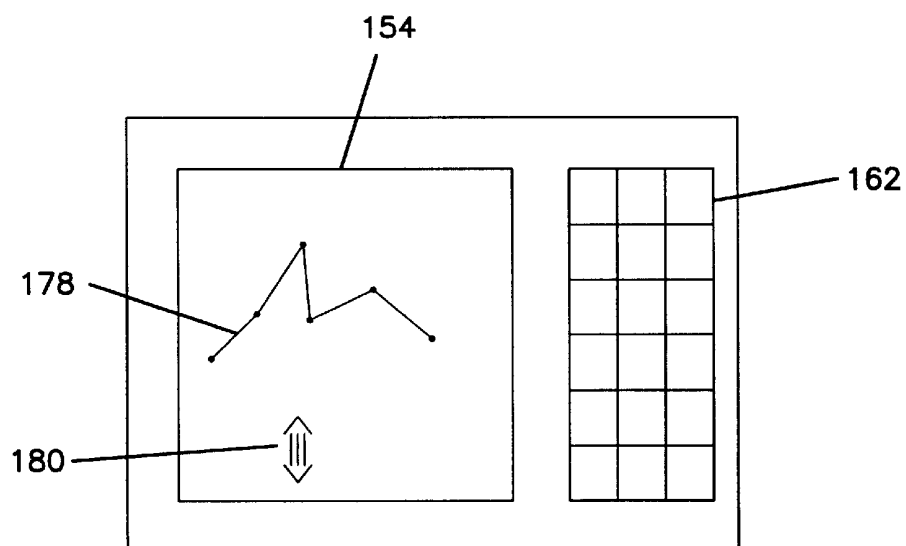


FIG. 25

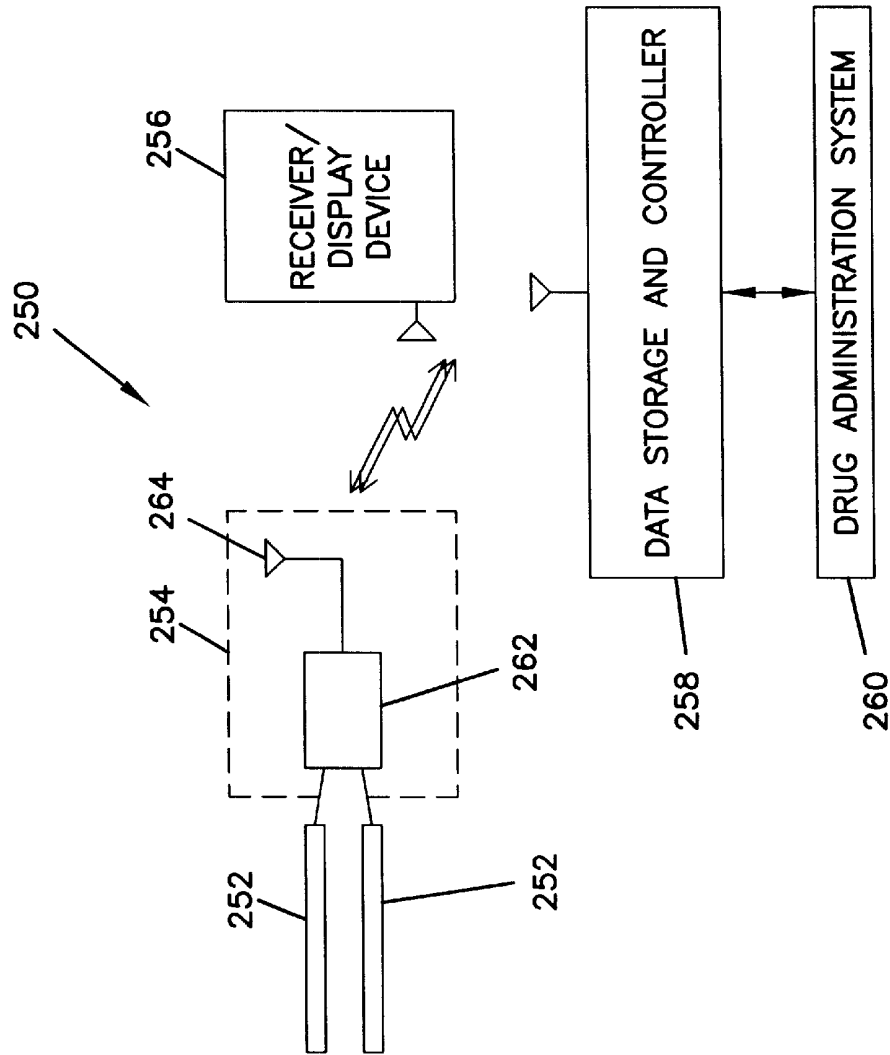

U.S. Patent

May 20, 2003

Sheet 19 of 26

US 6,565,509 B1

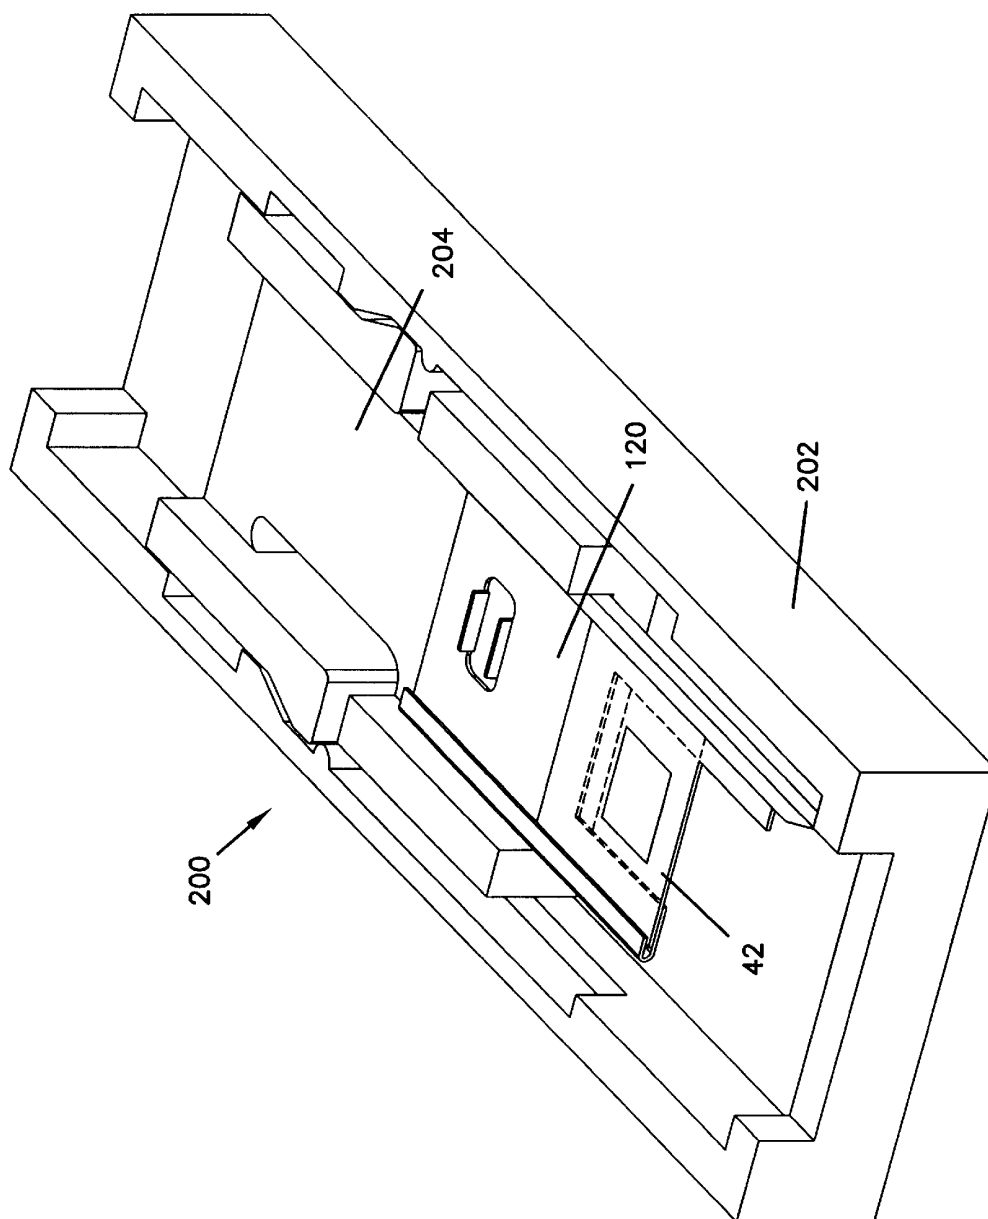



FIG. 26

U.S. Patent

May 20, 2003

Sheet 20 of 26

US 6,565,509 B1

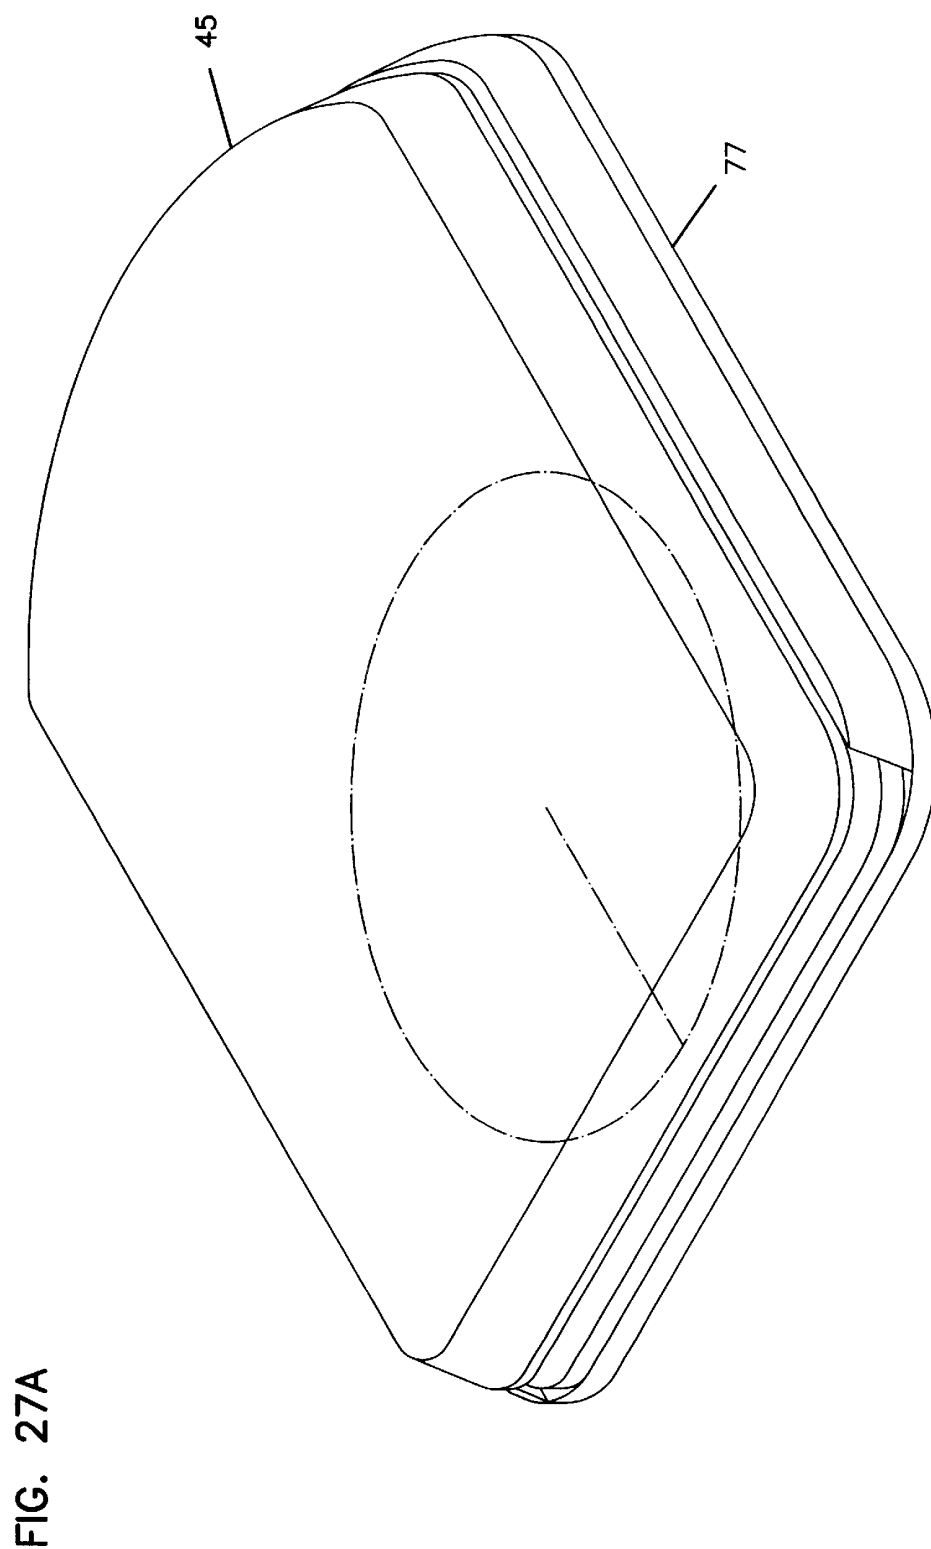

U.S. Patent

May 20, 2003

Sheet 21 of 26

US 6,565,509 B1

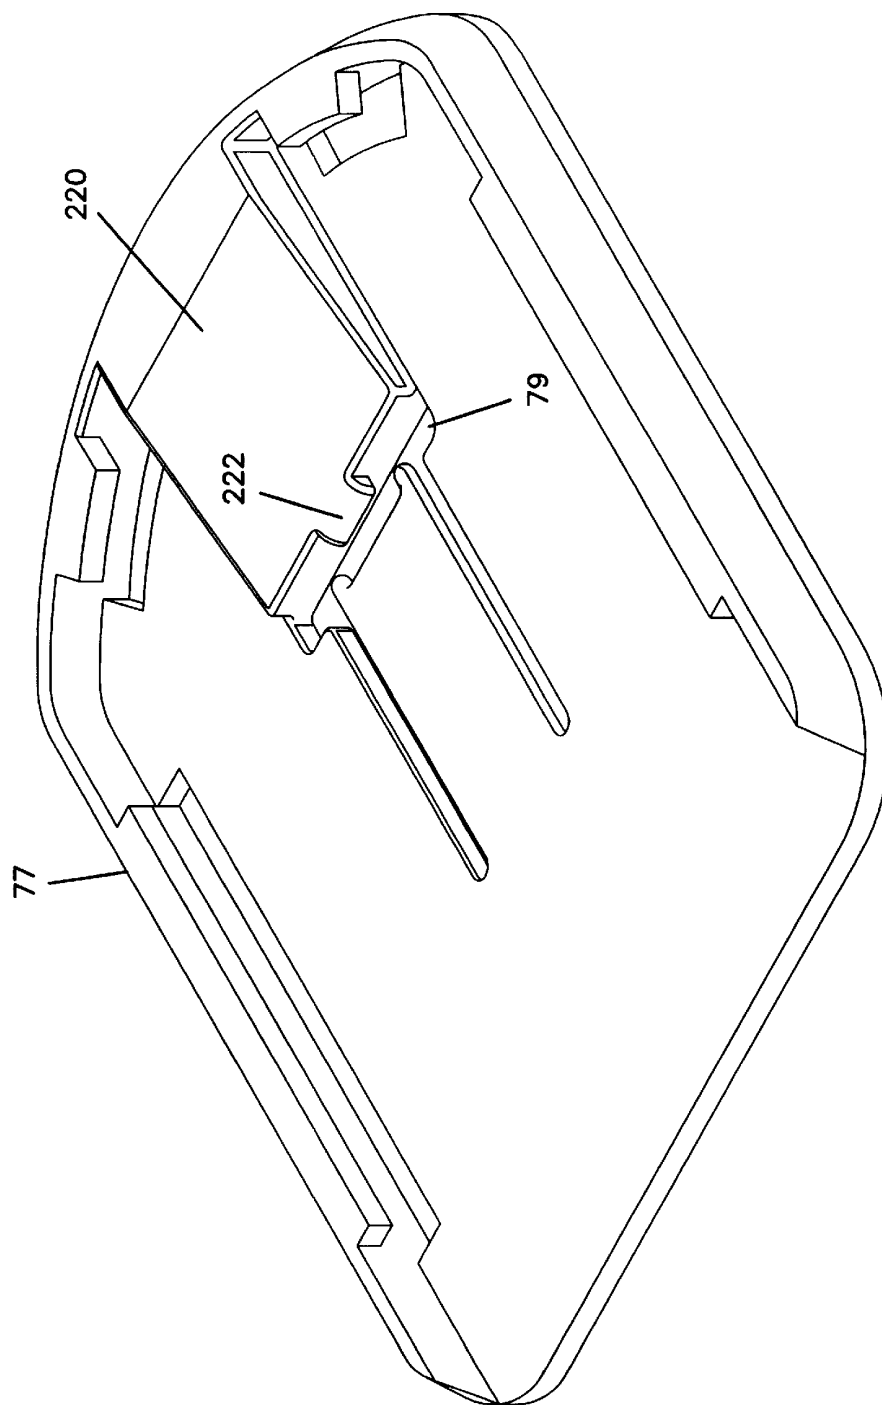


FIG. 27B

U.S. Patent

May 20, 2003

Sheet 22 of 26

US 6,565,509 B1

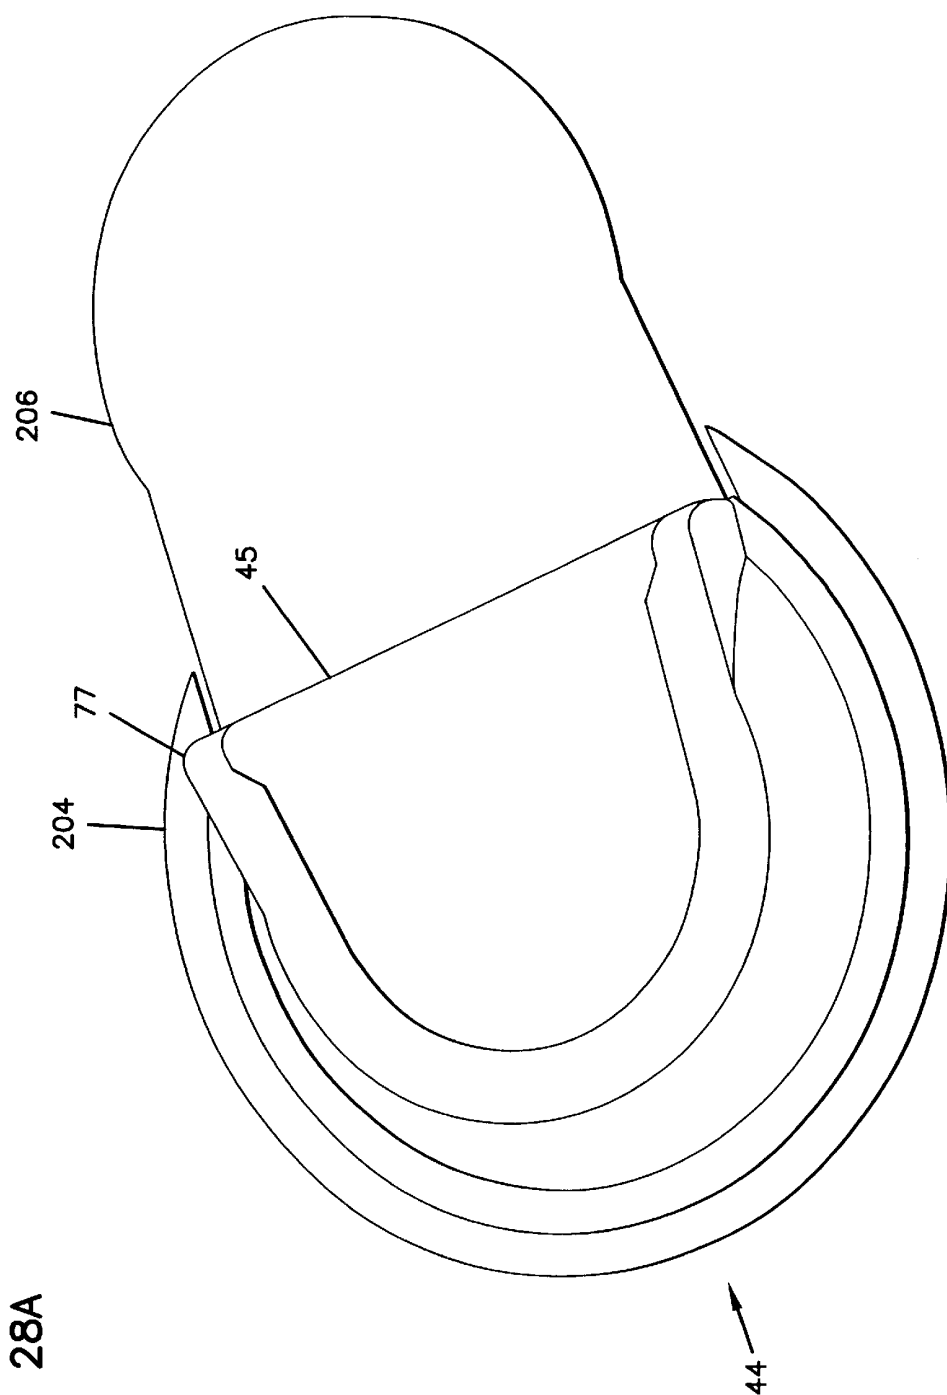


FIG. 28A

U.S. Patent

May 20, 2003

Sheet 23 of 26

US 6,565,509 B1

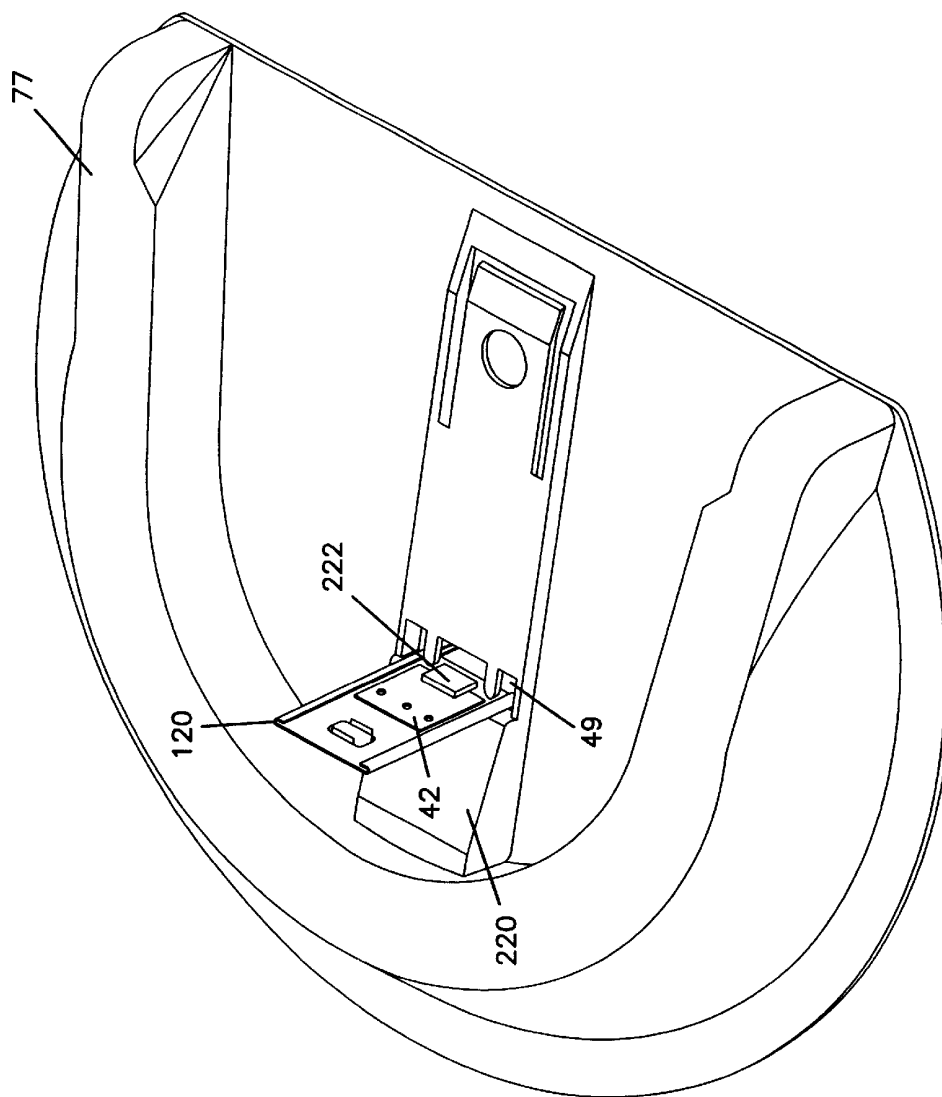


FIG. 28B

U.S. Patent

May 20, 2003

Sheet 24 of 26

US 6,565,509 B1

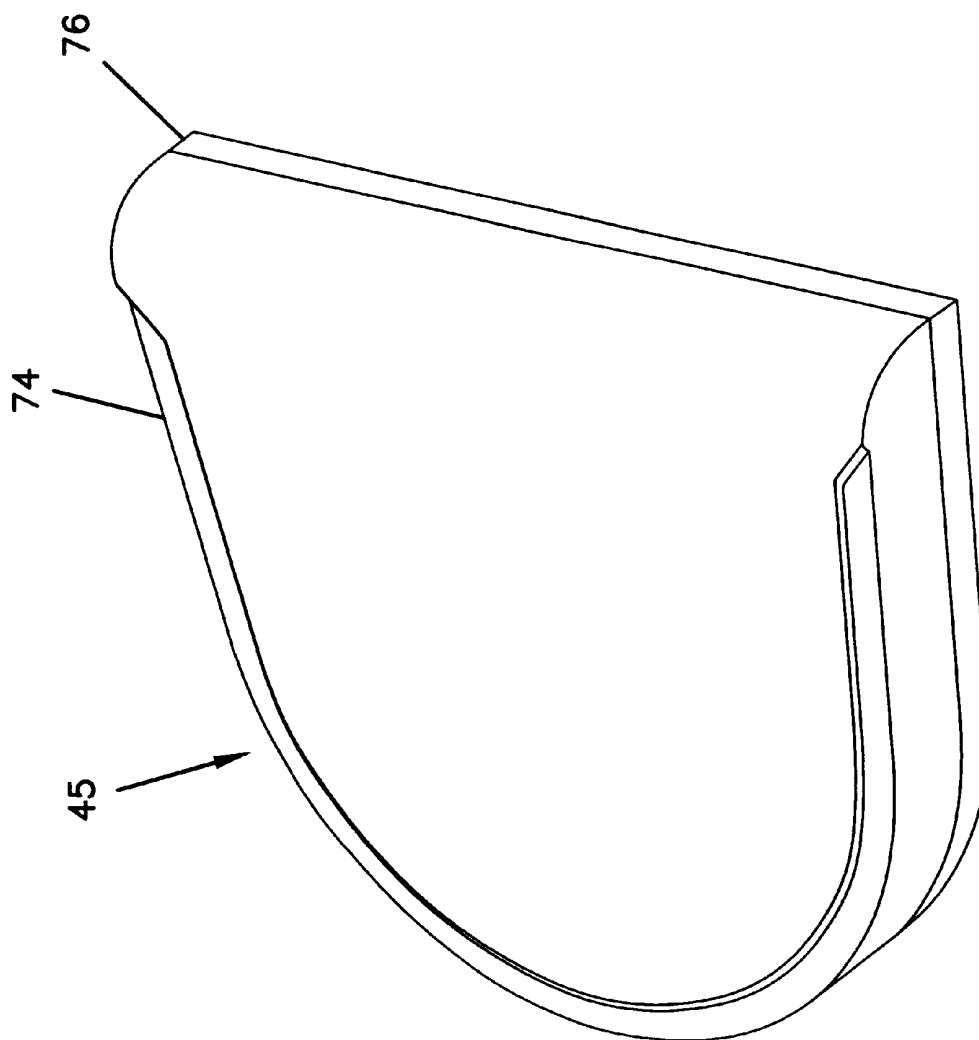


FIG. 28C

U.S. Patent

May 20, 2003

Sheet 25 of 26

US 6,565,509 B1

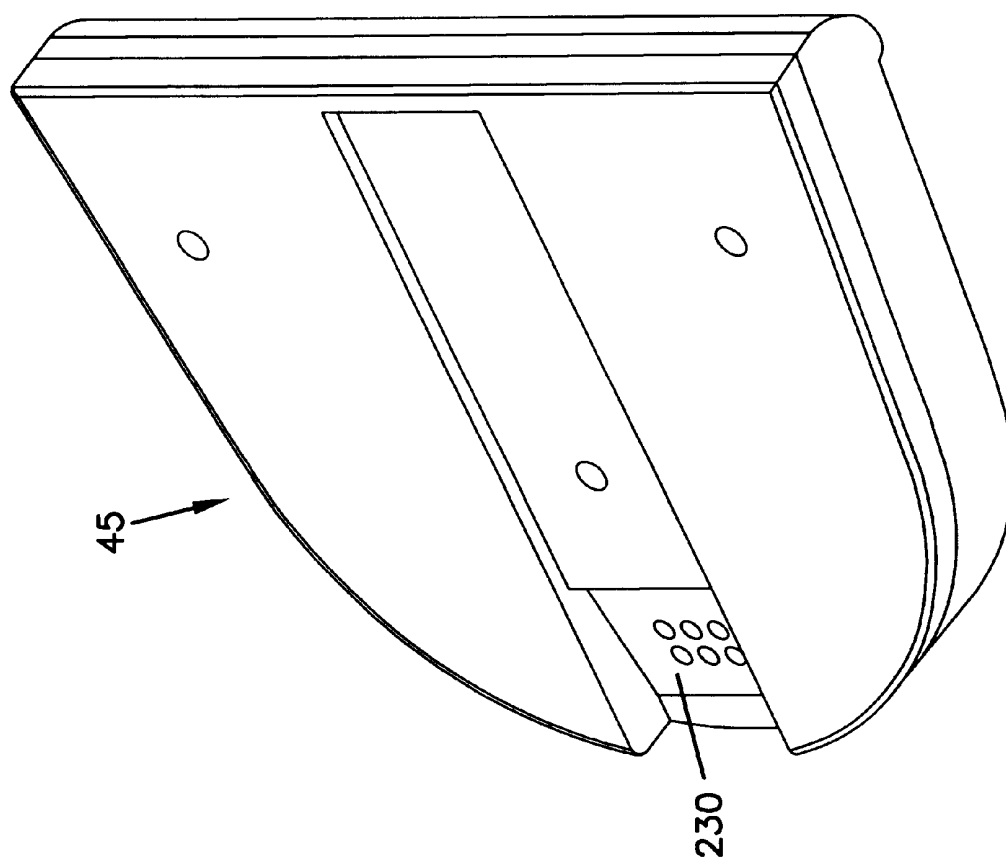


FIG. 28D

U.S. Patent

May 20, 2003

Sheet 26 of 26

US 6,565,509 B1

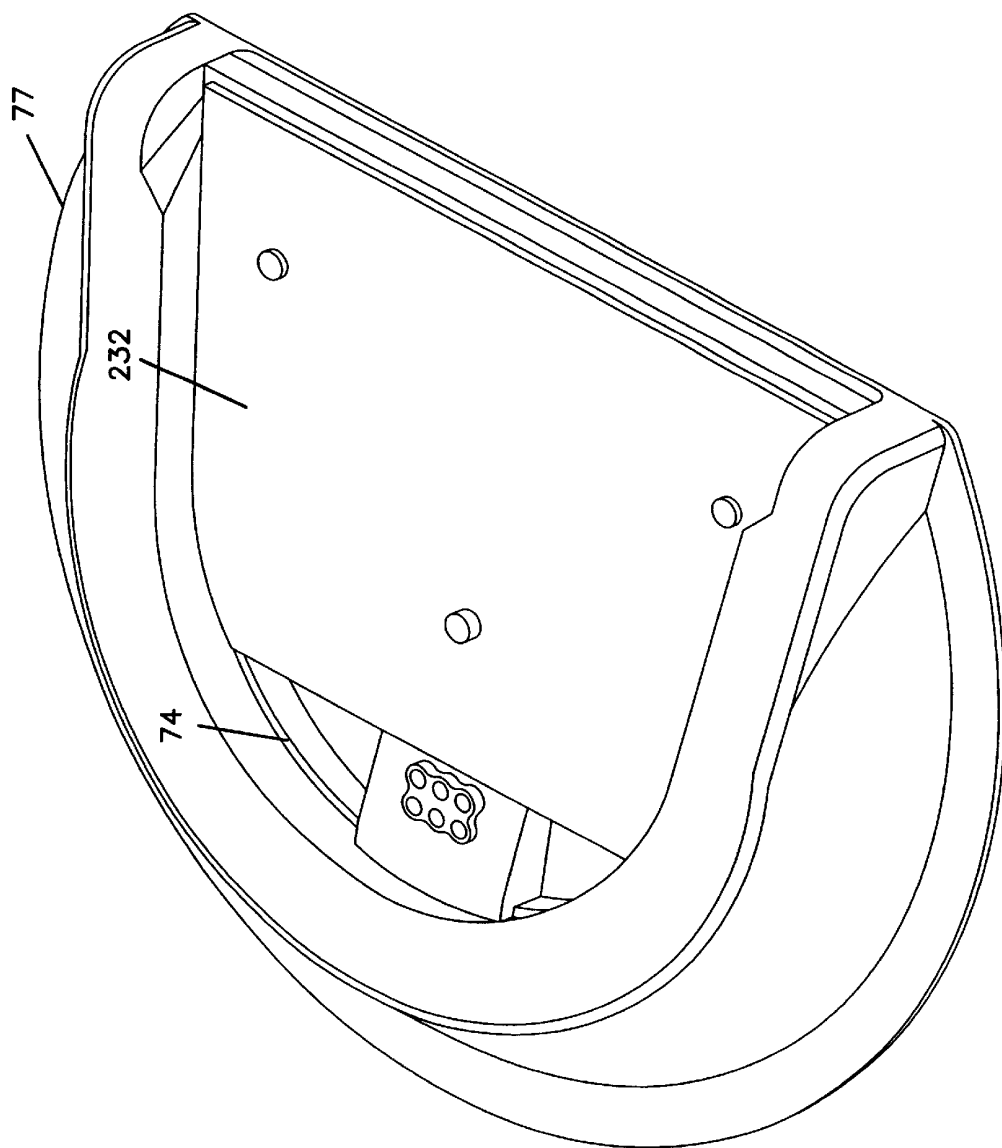


FIG. 28E

US 6,565,509 B1

1

**ANALYTE MONITORING DEVICE AND
METHODS OF USE**

This application is a continuation of application Ser. No. 09/070,677, filed Apr. 30, 1998, which is incorporated herein by reference.

FIELD OF THE INVENTION

The present invention is, in general, directed to devices and methods for the in vivo monitoring of an analyte, such as glucose or lactate. More particularly, the present invention relates to devices and methods for the in vivo monitoring of an analyte using an electrochemical sensor to provide information to a patient about the level of the analyte.

BACKGROUND OF THE INVENTION

The monitoring of the level of glucose or other analytes, such as lactate or oxygen, in certain individuals is vitally important to their health. High or low levels of glucose or other analytes may have detrimental effects. The monitoring of glucose is particularly important to individuals with diabetes, as they must determine when insulin is needed to reduce glucose levels in their bodies or when additional glucose is needed to raise the level of glucose in their bodies.

A conventional technique used by many diabetics for personally monitoring their blood glucose level includes the periodic drawing of blood, the application of that blood to a test strip, and the determination of the blood glucose level using colorimetric, electrochemical, or photometric detection. This technique does not permit continuous or automatic monitoring of glucose levels in the body, but typically must be performed manually on a periodic basis. Unfortunately, the consistency with which the level of glucose is checked varies widely among individuals. Many diabetics find the periodic testing inconvenient and they sometimes forget to test their glucose level or do not have time for a proper test. In addition, some individuals wish to avoid the pain associated with the test. These situations may result in hyperglycemic or hypoglycemic episodes. An in vivo glucose sensor that continuously or automatically monitors the individual's glucose level would enable individuals to more easily monitor their glucose, or other analyte, levels.

A variety of devices have been developed for continuous or automatic monitoring of analytes, such as glucose, in the blood stream or interstitial fluid. A number of these devices use electrochemical sensors which are directly implanted into a blood vessel or in the subcutaneous tissue of a patient. However, these devices are often difficult to reproducibly and inexpensively manufacture in large numbers. In addition, these devices are typically large, bulky, and/or inflexible, and many can not be used effectively outside of a controlled medical facility, such as a hospital or a doctor's office, unless the patient is restricted in his activities.

Some devices include a sensor guide which rests on or near the skin of the patient and may be attached to the patient to hold the sensor in place. These sensor guides are typically bulky and do not allow for freedom of movement. In addition, the sensor guides or the sensors include cables or wires for connecting the sensor to other equipment to direct the signals from the sensors to an analyzer. The size of the sensor guides and presence of cables and wires hinders the convenient use of these devices for everyday applications. There is a need for a small, compact device that can operate the sensor and provide signals to an analyzer without substantially restricting the movements and activities of a patient.

2

The patient's comfort and the range of activities that can be performed while the sensor is implanted are important considerations in designing extended-use sensors for continuous or automatic in vivo monitoring of the level of an analyte, such as glucose. There is a need for a small, comfortable device which can continuously monitor the level of an analyte, such as glucose, while still permitting the patient to engage in normal activities. Continuous and/or automatic monitoring of the analyte can provide a warning to the patient when the level of the analyte is at or near a threshold level. For example, if glucose is the analyte, then the monitoring device might be configured to warn the patient of current or impending hyperglycemia or hypoglycemia. The patient can then take appropriate actions.

SUMMARY OF THE INVENTION

Generally, the present invention relates to methods and devices for the continuous and/or automatic in vivo monitoring of the level of an analyte using a subcutaneously implantable sensor. Many of these devices are small and comfortable when used, thereby allowing a wide range of activities. One embodiment is a sensor control unit having a housing adapted for placement on skin. The housing is also adapted to receive a portion of an electrochemical sensor. The sensor control unit includes two or more conductive contacts disposed on the housing and configured for coupling to two or more contact pads on the sensor. A transmitter is disposed in the housing and coupled to the plurality of conductive contacts for transmitting data obtained using the sensor. The sensor control unit may also include a variety of optional components, such as, for example, adhesive for adhering to the skin, a mounting unit, a receiver, a processing circuit, a power supply (e.g., a battery), an alarm system, a data storage unit, a watchdog circuit, and a measurement circuit. Other optional components are described below.

Another embodiment of the invention is a sensor assembly that includes the sensor control unit described above. The sensor assembly also includes a sensor having at least one working electrode and at least one contact pad coupled to the working electrode or electrodes. The sensor may also include optional components, such as, for example, a counter electrode, a counter/reference electrode, a reference electrode, and a temperature probe. Other components and options for the sensor are described below.

A further embodiment of the invention is an analyte monitoring system that includes the sensor control unit described above. The analyte monitoring system also includes a sensor that has at least one working electrode and at least one contact pad coupled to the working electrode or electrodes. The analyte monitoring system also includes a display unit that has a receiver for receiving data from the sensor control unit and a display coupled to the receiver for displaying an indication of the level of an analyte. The display unit may optionally include a variety of components, such as, for example, a transmitter, an analyzer, a data storage unit, a watchdog circuit, an input device, a power supply, a clock, a lamp, a pager, a telephone interface, a computer interface, an alarm or alarm system, a radio, and a calibration unit. Further components and options for the display unit are described below. In addition, the analyte monitoring system or a component of the analyte monitoring system may optionally include a processor capable of determining a drug or treatment protocol and/or a drug delivery system.

Yet another embodiment of the invention is an insertion kit for inserting an electrochemical sensor into a patient. The

US 6,565,509 B1

3

insertion kit includes an inserter. A portion of the inserter has a sharp, rigid, planer structure adapted to support the sensor during insertion of the electrochemical sensor. The insertion kit also includes an insertion gun having a port configured to accept the electrochemical sensor and the inserter. The insertion gun has a driving mechanism for driving the inserter and electrochemical sensor into the patient, and a retraction mechanism for removing the inserter while leaving the sensor within the patient.

Another embodiment is a method of using an electrochemical sensor. A mounting unit is adhered to skin of a patient. An insertion gun is aligned with a port on the mounting unit. The electrochemical sensor is disposed within the insertion gun and then the electrochemical sensor is inserted into the skin of the patient using the insertion gun. The insertion gun is removed and a housing of the sensor control unit is mounted on the mounting base. A plurality of conductive contacts disposed on the housing is coupled to a plurality of contact pads disposed on the electrochemical sensor to prepare the sensor for use.

One embodiment of the invention is a method for detecting failures in an implanted analyte-responsive sensor. An analyte-responsive sensor is implanted into a patient. The analyte-responsive sensor includes N working electrodes, where N is an integer and is two or greater, and a common counter electrode. Signals generated at one of the N working electrodes and at the common counter electrode are then obtained and the sensor is determined to have failed if the signal from the common counter electrode is not N times the signal from one of the working electrodes, within a predetermined threshold limit.

Yet another embodiment is a method of calibrating an electrochemical sensor having one or more working electrodes implanted in a patient. A signal is generated from each of the working electrodes. Several conditions are tested to determine if calibration is appropriate. First, the signals from each of the one or more working electrodes should differ by less than a first threshold amount. Second, the signals from each of the one or more working electrodes should be within a predetermined range. And, third, a rate of change of the signals from each of the one or more working electrodes should be less than a second threshold amount. A calibration value is found assaying a calibration sample of a patient's body fluid. The calibration value is then related to at least one of the signals from the one or more working electrodes if the conditions described above are met.

A further embodiment is a method for monitoring a level of an analyte. A sensor is inserted into a skin of a patient and a sensor control unit is attached to the skin of the patient. Two or more conductive contacts on the sensor control unit are coupled to contact pads on the sensor. Then, using the sensor control unit, data is collected regarding a level of an analyte from signals generated by the sensor. The collected data is transmitted to a display unit and an indication of the level of the analyte is displayed on the display unit.

The above summary of the present invention is not intended to describe each disclosed embodiment or every implementation of the present invention. The Figures and the detailed description which follow more particularly exemplify these embodiments.

BRIEF DESCRIPTION OF THE DRAWINGS

The invention may be more completely understood in consideration of the following detailed description of various embodiments of the invention in connection with the accompanying drawings, in which:

4

FIG. 1 is a block diagram of one embodiment of a subcutaneous analyte monitor using a subcutaneously implantable analyte sensor, according to the invention;

FIG. 2 is a top view of one embodiment of an analyte sensor, according to the invention;

FIG. 3A is a cross-sectional view of the analyte sensor of FIG. 2;

FIG. 3B is a cross-sectional view of another embodiment of an analyte sensor, according to the invention;

FIG. 4A is a cross-sectional view of a third embodiment of an analyte sensor, according to the invention;

FIG. 4B is a cross-sectional view of a fourth embodiment of an analyte sensor, according to the invention;

FIG. 5 is an expanded top view of a tip portion of the analyte sensor of FIG. 2;

FIG. 6 is a cross-sectional view of a fifth embodiment of an analyte sensor, according to the invention;

FIG. 7 is an expanded top view of a tip-portion of the analyte sensor of FIG. 6;

FIG. 8 is an expanded bottom view of a tip-portion of the analyte sensor of FIG. 6;

FIG. 9 is a side view of the analyte sensor of FIG. 2;

FIG. 10 is a top view of the analyte sensor of FIG. 6;

FIG. 11 is a bottom view of the analyte sensor of FIG. 6;

FIG. 12 is an expanded side view of one embodiment of a sensor and an insertion device, according to the invention;

FIGS. 13A, 13B, 13C are cross-sectional views of three embodiments of the insertion device of FIG. 12;

FIG. 14 is a cross-sectional view of one embodiment of a on-skin sensor control unit, according to the invention;

FIG. 15 is a top view of a base of the on-skin sensor control unit of FIG. 14;

FIG. 16 is a bottom view of a cover of the on-skin sensor control unit of FIG. 14;

FIG. 17 is a perspective view of the on-skin sensor control unit of FIG. 14 on the skin of a patient;

FIG. 18A is a block diagram of one embodiment of an on-skin sensor control unit, according to the invention;

FIG. 18B is a block diagram of another embodiment of an on-skin sensor control unit, according to the invention;

FIGS. 19A, 19B, 19C, and 19D are cross-sectional views of four embodiments of conductive contacts disposed on an interior surface of a housing of an on-skin sensor control unit, according to the invention;

FIGS. 19E and 19F are cross-sectional views of two embodiments of conductive contacts disposed on an exterior surface of a housing of an on-skin sensor control unit, according to the invention;

FIGS. 20A and 20B are schematic diagrams of two embodiments of a current-to-voltage converter for use in an analyte monitoring device, according to the invention;

FIG. 21 is a block diagram of one embodiment of an open loop modulation system for use in an analyte monitoring device, according to the invention;

FIG. 22 is a block diagram of one embodiment of a receiver/display unit, according to the invention;

FIG. 23 is a front view of one embodiment of a receiver/display unit;

FIG. 24 is a front view of a second embodiment of a receiver/display unit;

FIG. 25 is a block diagram of one embodiment of a drug delivery system, according to the invention;

US 6,565,509 B1

5

FIG. 26 is a perspective view of the internal structure of an insertion gun, according to the invention;

FIG. 27A is a top view of one embodiment of an on-skin sensor control unit, according to the invention;

FIG. 27B is a top view of one embodiment of a mounting unit of the on-skin sensor control unit of FIG. 27A;

FIG. 28A is a top view of another embodiment of an on-skin sensor control unit after insertion of an insertion device and a sensor, according to the invention;

FIG. 28B is a top view of one embodiment of a mounting unit of the on-skin sensor control unit of FIG. 28A;

FIG. 28C is a top view of one embodiment of a housing for at least a portion of the electronics of the on-skin sensor control unit of FIG. 28A;

FIG. 28D is a bottom view of the housing of FIG. 28C; and

FIG. 28E is a top view of the on-skin sensor control unit of FIG. 28A with a cover of the housing removed.

While the invention is amenable to various modifications and alternative forms, specifics thereof have been shown by way of example in the drawings and will be described in detail. It should be understood, however, that the intention is not to limit the invention to the particular embodiments described. On the contrary, the intention is to cover all modifications, equivalents, and alternatives falling within the spirit and scope of the invention as defined by the appended claims.

DETAILED DESCRIPTION OF THE INVENTION

The present invention is applicable to an analyte monitoring system using an implantable sensor for the in vivo determination of a concentration of an analyte, such as glucose or lactate, in a fluid. The sensor can be, for example, subcutaneously implanted in a patient for the continuous or periodic monitoring an analyte in a patient's interstitial fluid. This can then be used to infer the glucose level in the patient's bloodstream. Other in vivo analyte sensors can be made, according to the invention, for insertion into a vein, artery, or other portion of the body containing fluid. The analyte monitoring system is typically configured for monitoring the level of the analyte over a time period which may range from days to weeks or longer.

The following definitions are provided for terms used herein:

A "counter electrode" refers to an electrode paired with the working electrode, through which passes a current equal in magnitude and opposite in sign to the current passing through the working electrode. In the context of the invention, the term "counter electrode" is meant to include counter electrodes which also function as reference electrodes (i.e., a counter/reference electrode).

An "electrochemical sensor" is a device configured to detect the presence and/or measure the level of an analyte in a sample via electrochemical oxidation and reduction reactions on the sensor. These reactions are transduced to an electrical signal that can be correlated to an amount, concentration, or level of an analyte in the sample.

"Electrolysis" is the electrooxidation or electroreduction of a compound either directly at an electrode or via one or more electron transfer agents.

A compound is "immobilized" on a surface when it is entrapped on or chemically bound to the surface.

A "non-leachable" or "non-releasable" compound or a compound that is "non-leachably disposed" is meant to

6

define a compound that is affixed on the sensor such that it does not substantially diffuse away from the working surface of the working electrode for the period in which the sensor is used (e.g., the period in which the sensor is implanted in a patient or measuring a sample).

Components are "immobilized" within a sensor, for example, when the components are covalently, ionically, or coordinatively bound to constituents of the sensor and/or are entrapped in a polymeric or sol-gel matrix or membrane which precludes mobility.

An "electron transfer agent" is a compound that carries electrons between the analyte and the working electrode, either directly, or in cooperation with other electron transfer agents. One example of an electron transfer agent is a redox mediator.

A "working electrode" is an electrode at which the analyte (or a second compound whose level depends on the level of the analyte) is electrooxidized or electroreduced with or without the agency of an electron transfer agent.

A "working surface" is that portion of the working electrode which is coated with or is accessible to the electron transfer agent and configured for exposure to an analyte-containing fluid.

A "sensing layer" is a component of the sensor which includes constituents that facilitate the electrolysis of the analyte. The sensing layer may include constituents such as an electron transfer agent, a catalyst which catalyzes a reaction of the analyte to produce a response at the electrode, or both. In some embodiments of the sensor, the sensing layer is non-leachably disposed in proximity to or on the working electrode.

A "non-corroding" conductive material includes non-metallic materials, such as carbon and conductive polymers.

Analyte Sensor Systems

The analyte monitoring systems of the present invention can be utilized under a variety of conditions. The particular configuration of a sensor and other units used in the analyte monitoring system may depend on the use for which the analyte monitoring system is intended and the conditions under which the analyte monitoring system will operate. One embodiment of the analyte monitoring system includes a sensor configured for implantation into a patient or user. For example, implantation of the sensor may be made in the arterial or venous systems for direct testing of analyte levels in blood. Alternatively, a sensor may be implanted in the interstitial tissue for determining the analyte level in interstitial fluid. This level may be correlated and/or converted to analyte levels in blood or other fluids. The site and depth of implantation may affect the particular shape, components, and configuration of the sensor. Subcutaneous implantation may be preferred, in some cases, to limit the depth of implantation of the sensor. Sensors may also be implanted in other regions of the body to determine analyte levels in other fluids. Examples of suitable sensor for use in the analyte monitoring systems of the invention are described in U.S. patent application, Ser. No. 09/034,372, incorporated herein by reference.

One embodiment of the analyte monitoring system 40 for use with an implantable sensor 42, and particularly for use with a subcutaneously implantable sensor, is illustrated in block diagram form in FIG. 1. The analyte monitoring system 40 includes, at minimum, a sensor 42, a portion of which is configured for implantation (e.g., subcutaneous, venous, or arterial implantation) into a patient, and a sensor control unit 44. The sensor 42 is coupled to the sensor control unit 44 which is typically attached to the skin of a

US 6,565,509 B1

7

patient. The sensor control unit **44** operates the sensor **42**, including, for example, providing a voltage across the electrodes of the sensor **42** and collecting signals from the sensor **42**. The sensor control unit **44** may evaluate the signals from the sensor **42** and/or transmit the signals to one or more optional receiver/display units **46, 48** for evaluation. The sensor control unit **44** and/or the receiver/display units **46, 48** may display or otherwise communicate the current level of the analyte. Furthermore, the sensor control unit **44** and/or the receiver/display units **46, 48** may indicate to the patient, via, for example, an audible, visual, or other sensory-stimulating alarm, when the level of the analyte is at or near a threshold level. In some embodiments, a electrical shock can be delivered to the patient as a warning through one of the electrodes or the optional temperature probe of the sensor. For example, if glucose is monitored then an alarm may be used to alert the patient to a hypoglycemic or hyperglycemic glucose level and/or to impending hypoglycemia or hyperglycemia.

The Sensor

A sensor **42** includes at least one working electrode **58** formed on a substrate **50**, as shown in FIG. 2. The sensor **42** may also include at least one counter electrode **60** (or counter/reference electrode) and/or at least one reference electrode **62** (see FIG. 8). The counter electrode **60** and/or reference electrode **62** may be formed on the substrate **50** or may be separate units. For example, the counter electrode and/or reference electrode may be formed on a second substrate which is also implanted in the patient or, for some embodiments of the implantable sensors, the counter electrode and/or reference electrode may be placed on the skin of the patient with the working electrode or electrodes being implanted into the patient. The use of an on-the-skin counter and/or reference electrode with an implantable working electrode is described in U.S. Pat. No. 5,593,852, incorporated herein by reference.

The working electrode or electrodes **58** are formed using conductive traces **52** disposed on the substrate **50**. The counter electrode **60** and/or reference electrode **62**, as well as other optional portions of the sensor **42**, such as a temperature probe **66** (see FIG. 8), may also be formed using conductive traces **52** disposed on the substrate **50**. These conductive traces **52** may be formed over a smooth surface of the substrate **50** or within channels **54** formed by, for example, embossing, indenting or otherwise creating a depression in the substrate **50**.

A sensing layer **64** (see FIGS. 3A and 3B) is often formed proximate to or on at least one of the working electrodes **58** to facilitate the electrochemical detection of the analyte and the determination of its level in the sample fluid, particularly if the analyte can not be electrolyzed at a desired rate and/or with a desired specificity on a bare electrode. The sensing layer **64** may include an electron transfer agent to transfer electrons directly or indirectly between the analyte and the working electrode **58**. The sensing layer **64** may also contain a catalyst to catalyze a reaction of the analyte. The components of the sensing layer may be in a fluid or gel that is proximate to or in contact with the working electrode **58**. Alternatively, the components of the sensing layer **64** may be disposed in a polymeric or sol-gel matrix that is proximate to or on the working electrode **58**. Preferably, the components of the sensing layer **64** are non-leachably disposed within the sensor **42**. More preferably, the components of the sensor **42** are immobilized within the sensor **42**.

In addition to the electrodes **58, 60, 62** and the sensing layer **64**, the sensor **42** may also include a temperature probe **66** (see FIGS. 6 and 8), a mass transport limiting layer **74**

8

(see FIG. 9), a biocompatible layer **75** (see FIG. 9), and/or other optional components, as described below. Each of these items enhances the functioning of and/or results from the sensor **42**, as discussed below.

The Substrate

The substrate **50** may be formed using a variety of non-conducting materials, including, for example, polymeric or plastic materials and ceramic materials. Suitable materials for a particular sensor **42** may be determined, at least in part, based on the desired use of the sensor **42** and properties of the materials.

In some embodiments, the substrate is flexible. For example, if the sensor **42** is configured for implantation into a patient, then the sensor **42** may be made flexible (although rigid sensors may also be used for implantable sensors) to reduce pain to the patient and damage to the tissue caused by the implantation of and/or the wearing of the sensor **42**. A flexible substrate **50** often increases the patient's comfort and allows a wider range of activities. Suitable materials for a flexible substrate **50** include, for example, non-conducting plastic or polymeric materials and other non-conducting, flexible, deformable materials. Examples of useful plastic or polymeric materials include thermoplastics such as polycarbonates, polyesters (e.g., Mylar™ and polyethylene terephthalate (PET)), polyvinyl chloride (PVC), polyurethanes, polyethers, polyamides, polyimides, or copolymers of these thermoplastics, such as PETG (glycol-modified polyethylene terephthalate).

In other embodiments, the sensors **42** are made using a relatively rigid substrate **50** to for example, provide structural support against bending or breaking. Examples of rigid materials that may be used as the substrate **50** include poorly conducting ceramics, such as aluminum oxide and silicon dioxide. One advantage of an implantable sensor **42** having a rigid substrate is that the sensor **42** may have a sharp point and/or a sharp edge to aid in implantation of a sensor **42** without an additional insertion device.

It will be appreciated that for many sensors **42** and sensor applications, both rigid and flexible sensors will operate adequately. The flexibility of the sensor **42** may also be controlled and varied along a continuum by changing, for example, the composition and/or thickness of the substrate **50**.

In addition to considerations regarding flexibility, it is often desirable that implantable sensors **42** should have a substrate **50** which is non-toxic. Preferably, the substrate **50** is approved by one or more appropriate governmental agencies or private groups for in vivo use.

The sensor **42** may include optional features to facilitate insertion of an implantable sensor **42**, as shown in FIG. 12. For example, the sensor **42** may be pointed at the tip **123** to ease insertion. In addition, the sensor **42** may include a barb **125** which assists in anchoring the sensor **42** within the tissue of the patient during operation of the sensor **42**. However, the barb **125** is typically small enough that little damage is caused to the subcutaneous tissue when the sensor **42** is removed for replacement.

Although the substrate **50** in at least some embodiments has uniform dimensions along the entire length of the sensor **42**, in other embodiments, the substrate **50** has a distal end **67** and a proximal end **65** with different widths **53, 55**, respectively, as illustrated in FIG. 2. In these embodiments, the distal end **67** of the substrate **50** may have a relatively narrow width **53**. For sensors **42** which are implantable into the subcutaneous tissue or another portion of a patient's body, the narrow width **53** of the distal end **67** of the substrate **50** may facilitate the implantation of the sensor **42**.